



K-Fridge
2024/6/3 08:53:52

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07539	1.06

Dataset parameters

Dataset name	Type of dataset
K-Fridge	Instant
Number of points	Interval
3167	15 minute(s)
Start date	End date
2024/5/1 09:20:00	2024/6/3 08:50:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 K□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.1	6.0	4.43
		Standard
		0.38
		MKT
		4.44

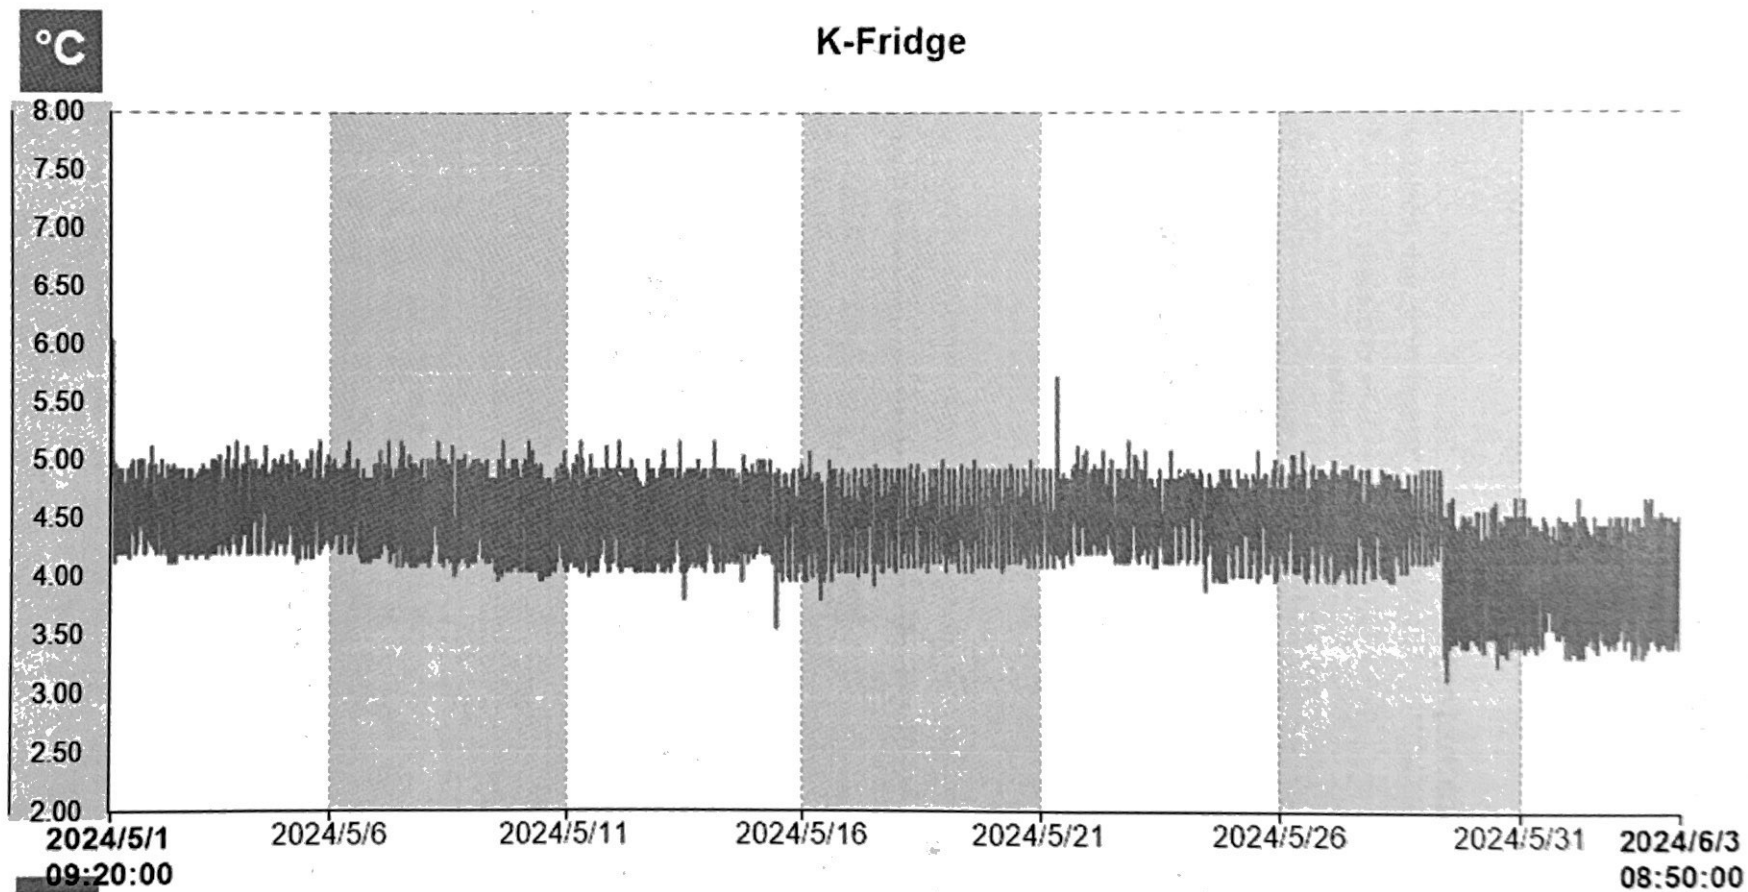



	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07539] Ch-int1 K... [°C]	3167	3.1	6.0	4.43	0.38	4.44