

Chih-I Wu
01 Aug 2024



K-Fridge back-up

2024/8/1 16:06:20

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07541	1.06

Dataset parameters

Dataset name	Type of dataset
K-Fridge back-up	Instant
Number of points	Interval
2612	15 minute(s)
Start date	End date
2024/7/5 11:05:00	2024/8/1 15:50:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 K-Fridge [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
2.6	4.9	3.89
		Standard
		0.48
		MKT
		3.90

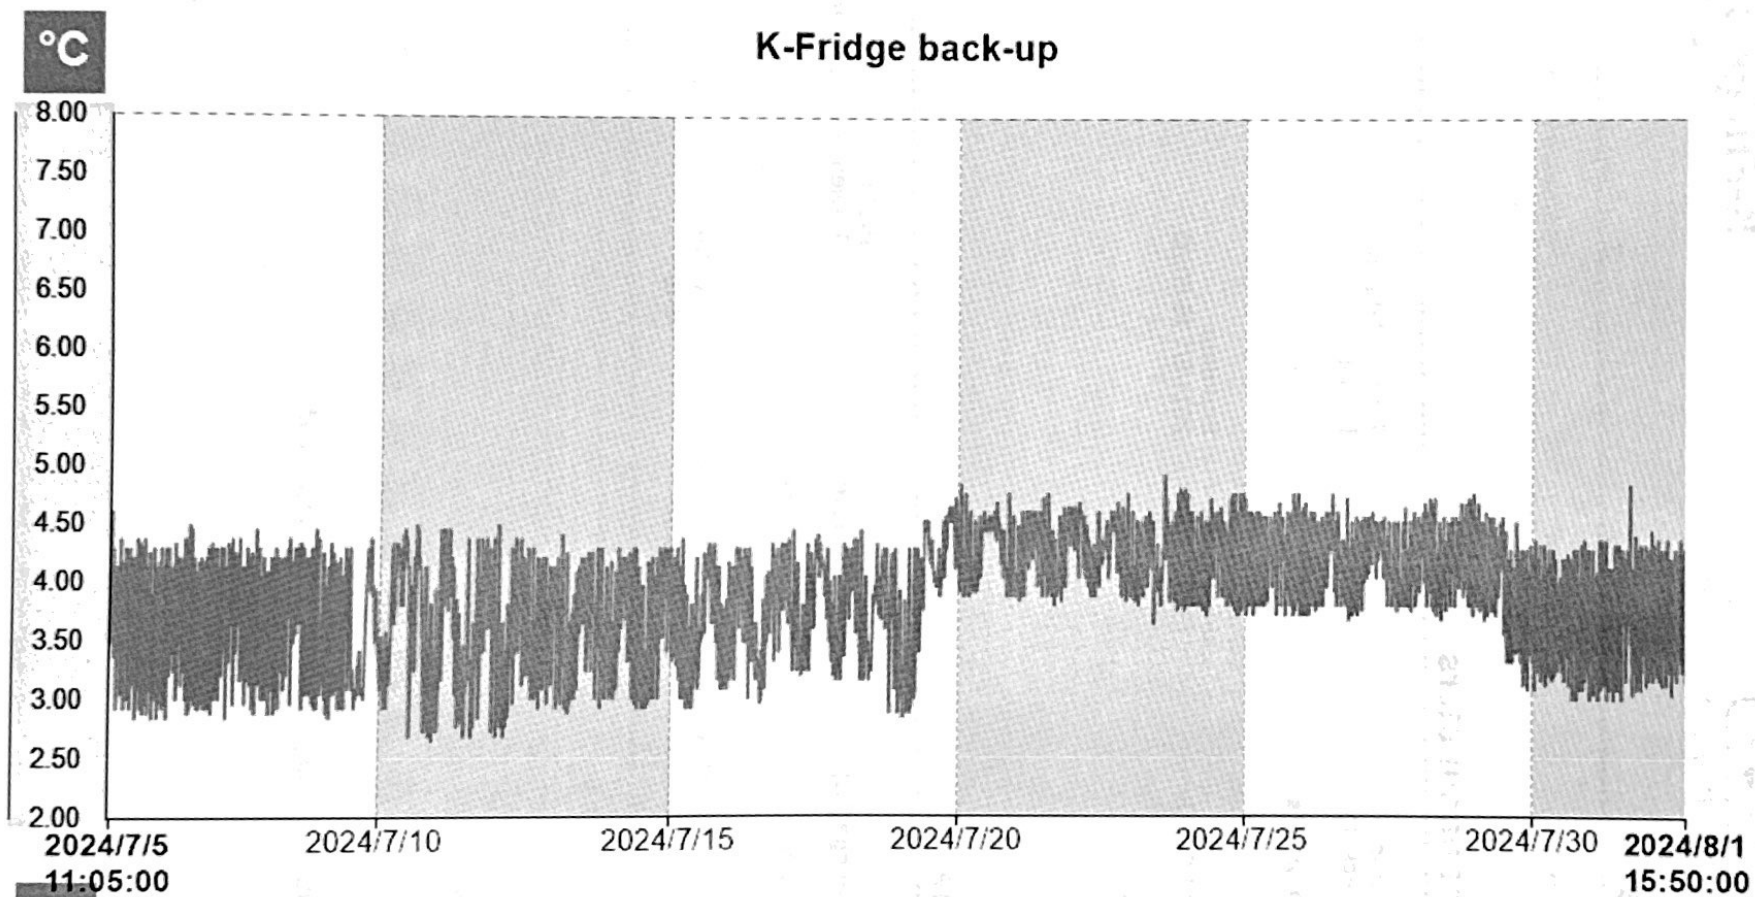



K-Fridge back-up

2024/8/1 16:06:20

		Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [0K 16.05.07541]	Ch-int1 K-Fridge [°C]	2612	2.6	4.9	3.89	0.48	3.90