



K-Fridge
2024/11/1 09:32:25

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07539	1.06

Dataset parameters

Dataset name	Type of dataset
K-Fridge	Instant
Number of points	Interval
2955	15 minute(s)
Start date	End date
2024/10/1 15:00:00	2024/11/1 09:30:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 K□□ [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
3.0	4.7	3.88	0.41	3.89

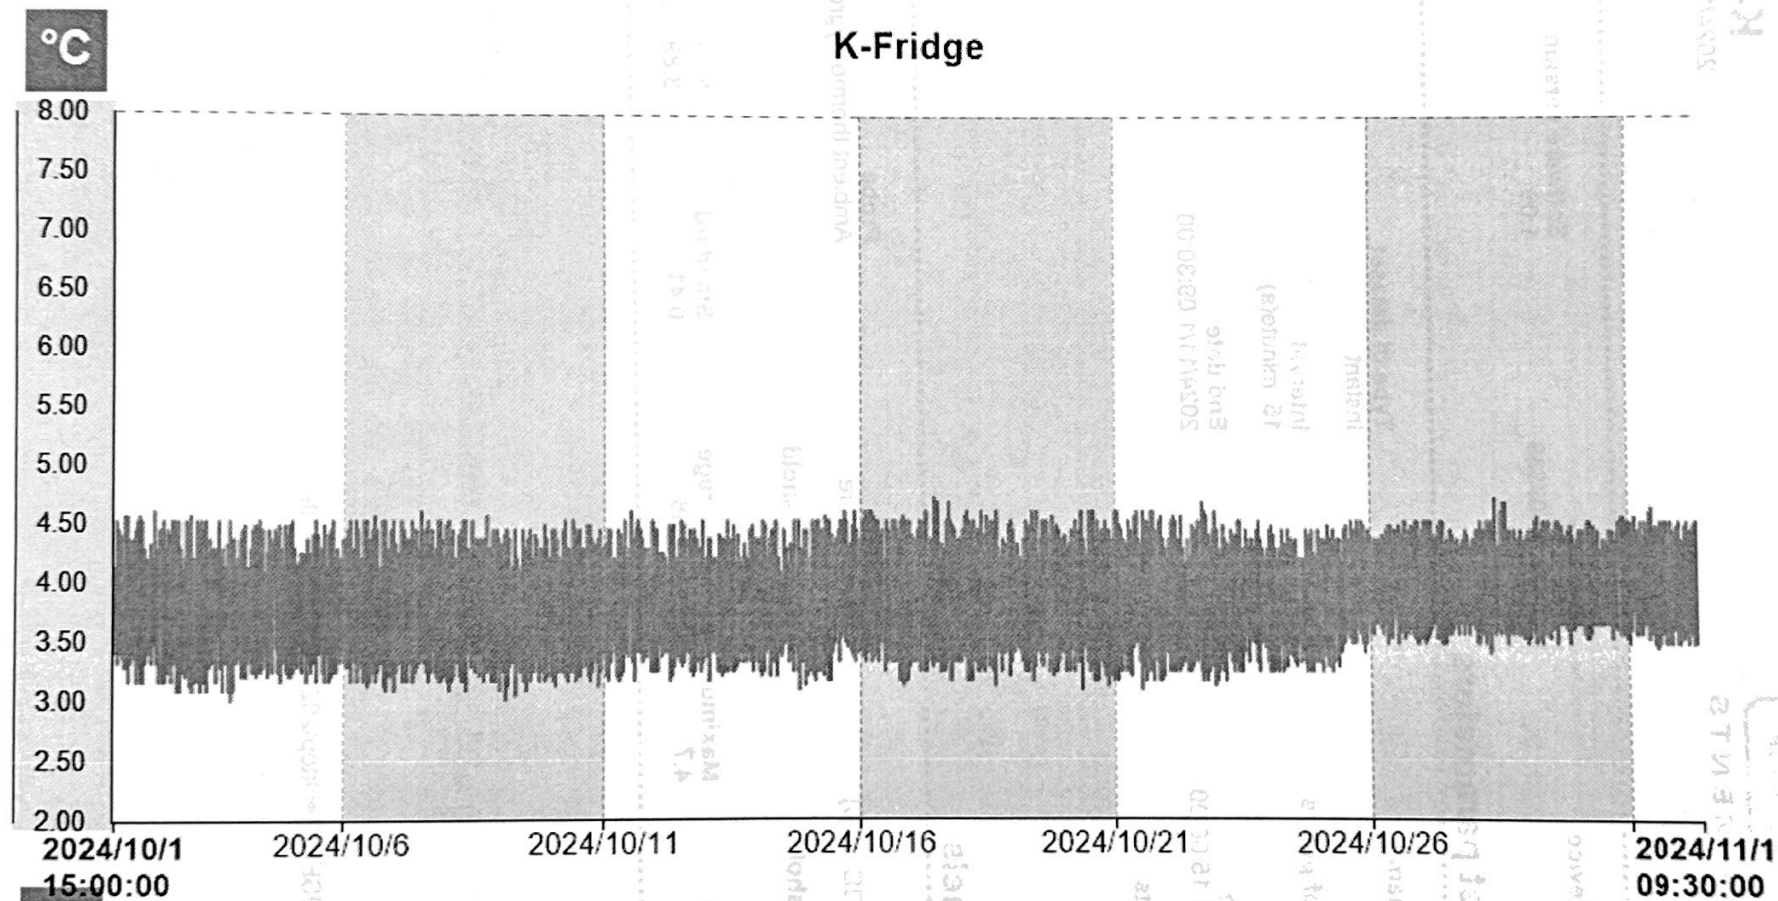



K-Fridge
2024/11/1 09:32:26

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [0K 16.05.07539]						
Ch-int1 K... [°C]	2955	3.0	4.7	3.88	0.41	3.89