



K-Fridge
2024/12/2 10:00:54

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07539	1.06

Dataset parameters

Dataset name	Type of dataset
K-Fridge	Instant
Number of points	Interval
2976	15 minute(s)
Start date	End date
2024/11/1 10:00:00	2024/12/2 09:45:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 K□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.0	5.2	3.89
		Standard
		0.40
		MKT
		3.90

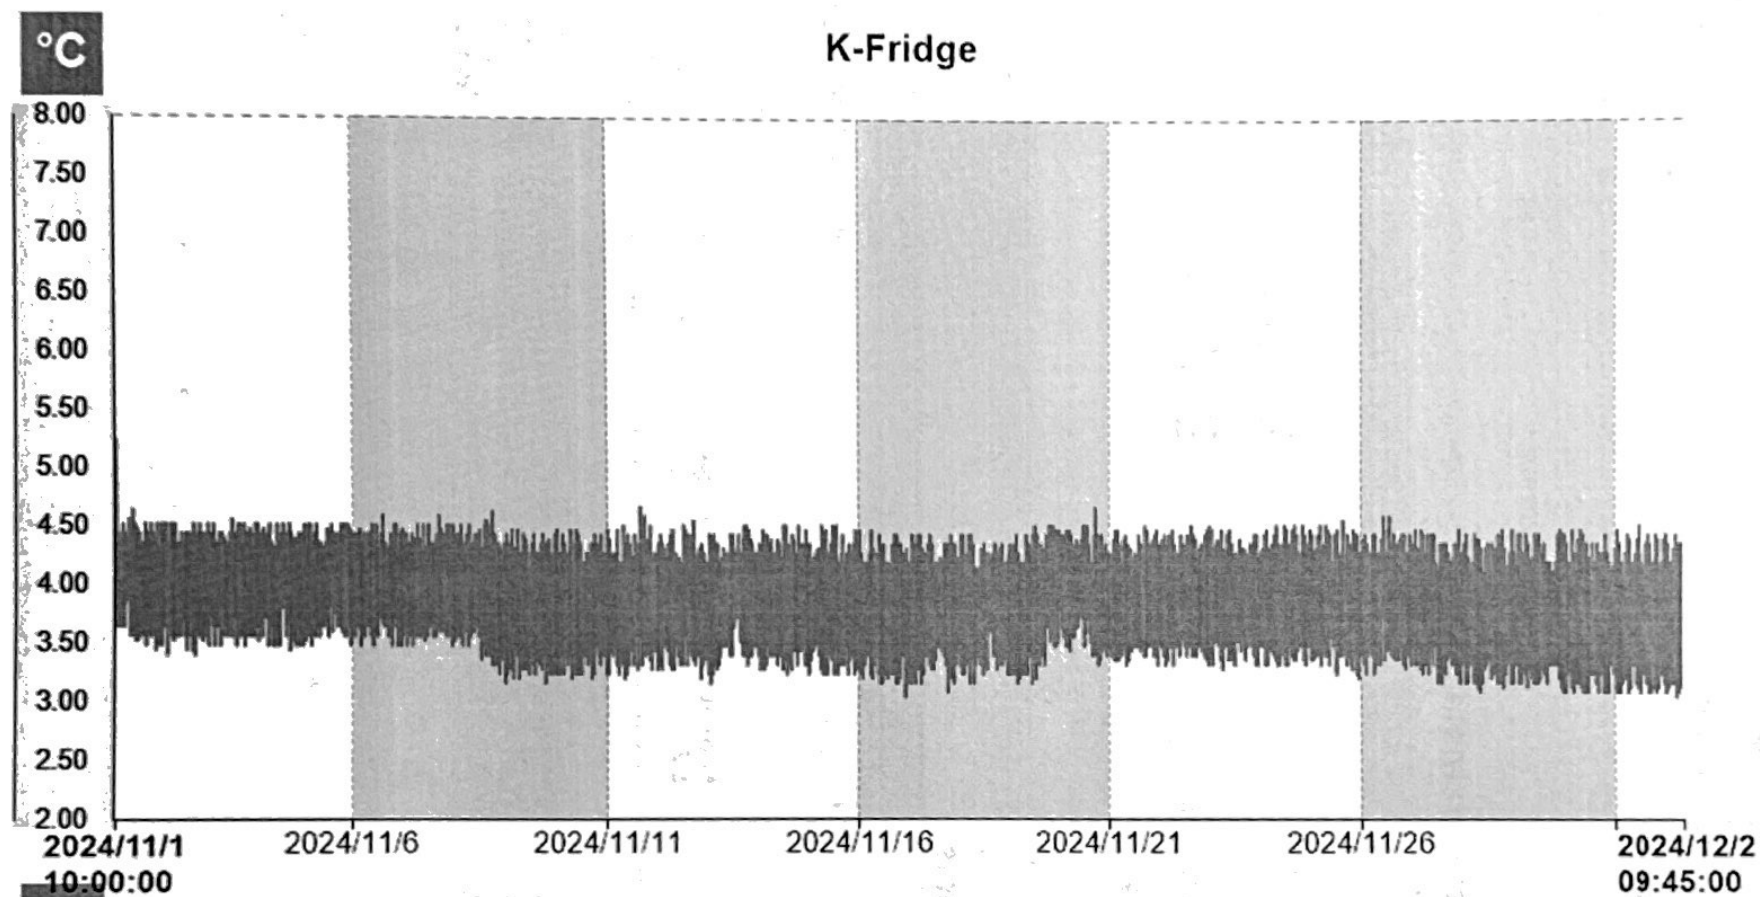



K-Fridge
2024/12/2 10:00:54

		Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07539]							
Ch-int1 K	[°C]	2976	3.0	5.2	3.89	0.40	3.90