



K-Fridge
2025/1/2 10:00:25

Device


Type of device	Serial n°	Software version
KH 50	0K 16.05.07539	1.06

Dataset parameters

Dataset name	Type of dataset
K-Fridge	Instant
Number of points	Interval
2975	15 minute(s)
Start date	End date
2024/12/2 10:20:00	2025/1/2 09:50:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 K□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
2.7	4.8	3.75
		Standard
		0.44
		MKT
		3.77

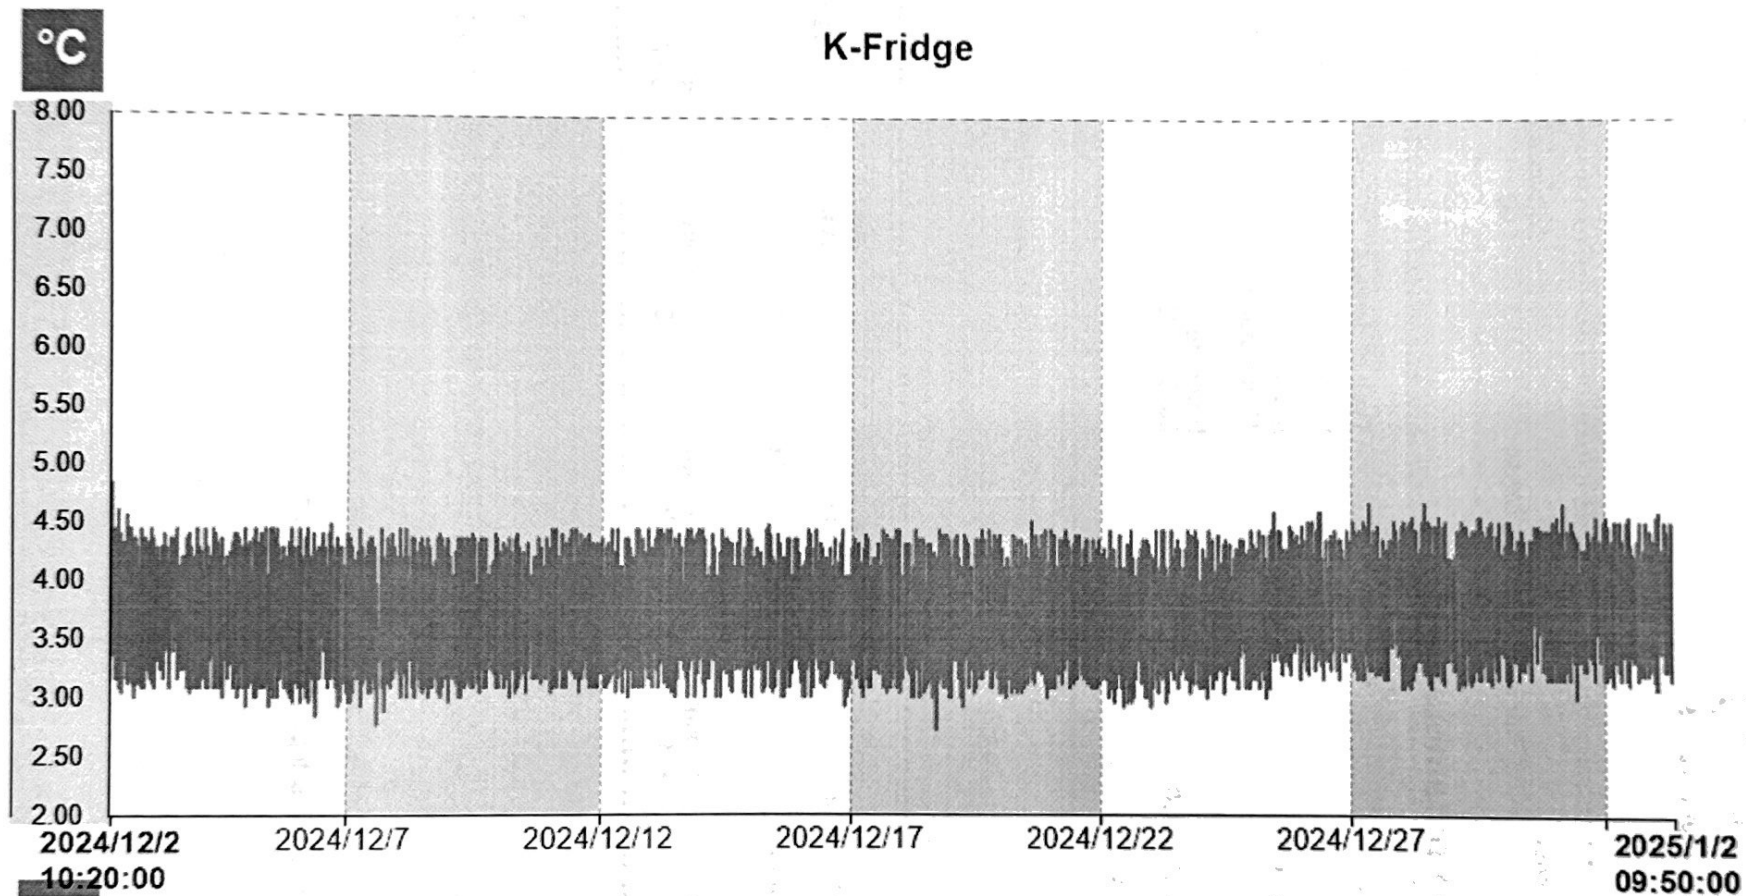



K-Fridge
2025/1/2 10:00:25

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [0K 16.05.07539]						
Ch-int1 K ₁₀₀ [°C]	2975	2.7	4.8	3.75	0.44	3.77