



K-Fridge
2025/2/3 10:23:45

Device

Type of device	Serial n°	Software version
KH 50	OK 16.05.07539	1.06


Dataset parameters

Dataset name	Type of dataset
K-Fridge	Instant
Number of points	Interval
3072	15 minute(s)
Start date	End date
2025/1/2 10:30:00	2025/2/3 10:15:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 K□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.0	5.0	3.94
		Standard
		0.32
		MKT
		3.95

2025/2/3 10:23:45
C:\Users\USER\Desktop\202501_K_Fridge.kfk

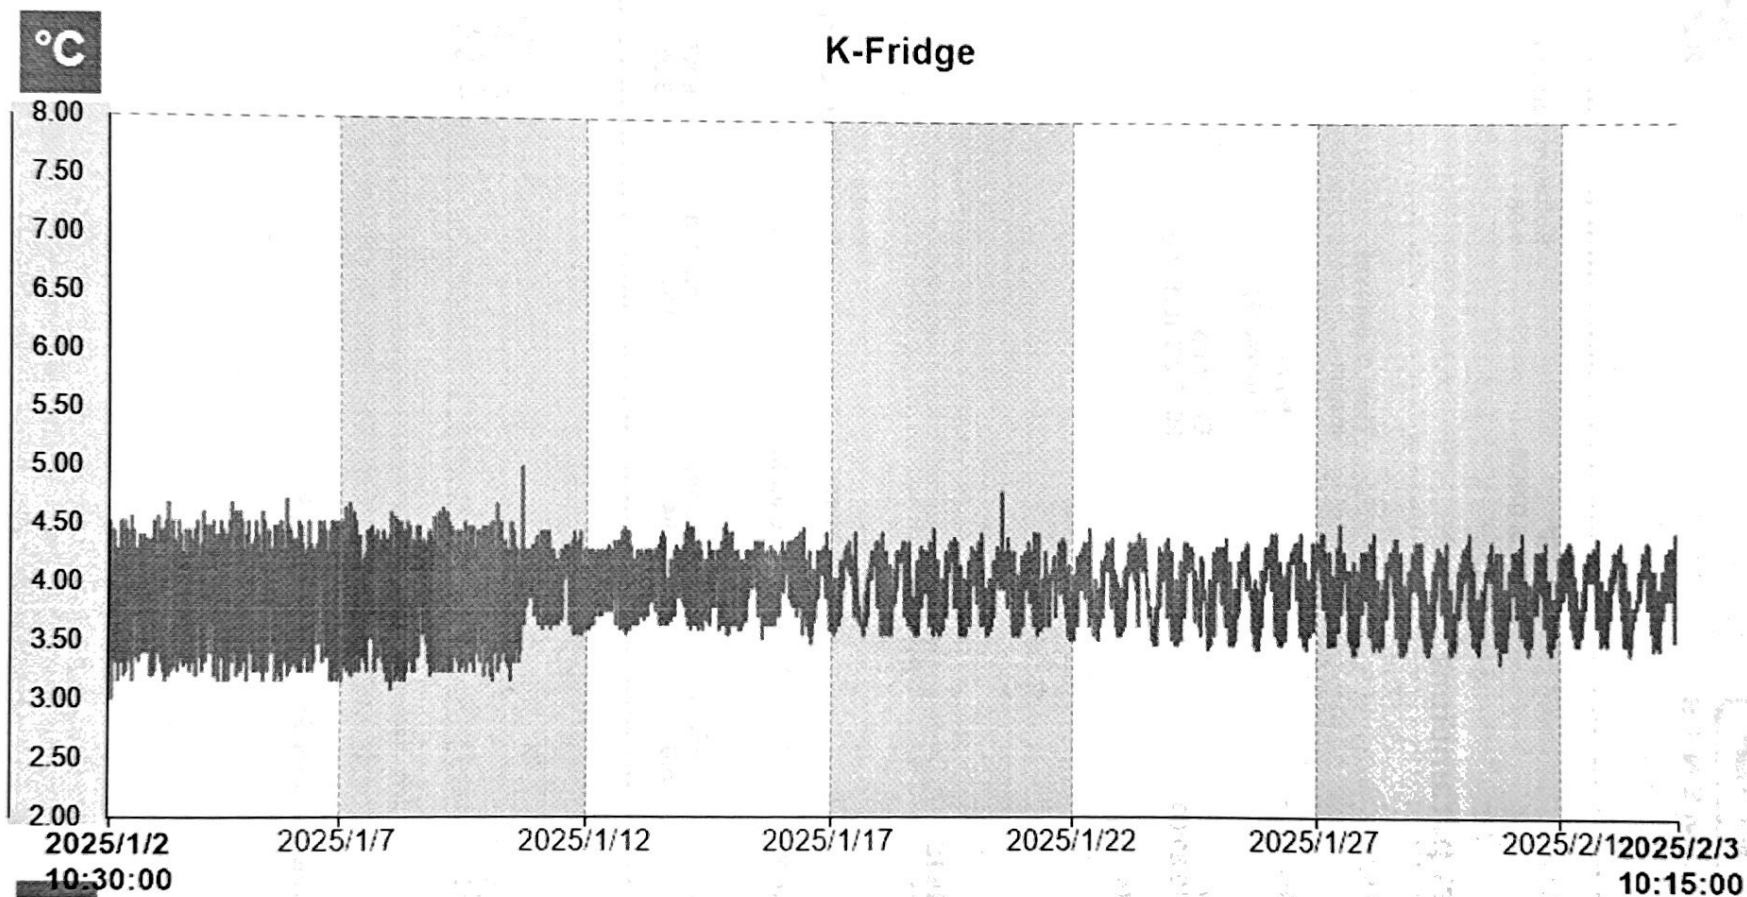



K-Fridge
2025/2/3 10:23:45

		Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07539]							
Ch-int1 K	[°C]	3072	3.0	5.0	3.94	0.32	3.95