

Chih-I Wu
02 Apr 2025



K-Fridge
2025/4/2 09:33:37

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07539	1.06

Dataset parameters

Dataset name	Type of dataset
K-Fridge	Instant
Number of points	Interval
2881	15 minute(s)
Start date	End date
2025/3/3 09:20:00	2025/4/2 09:20:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 K□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.0	4.8	3.97
		Standard
		0.41
		MKT
		3.98

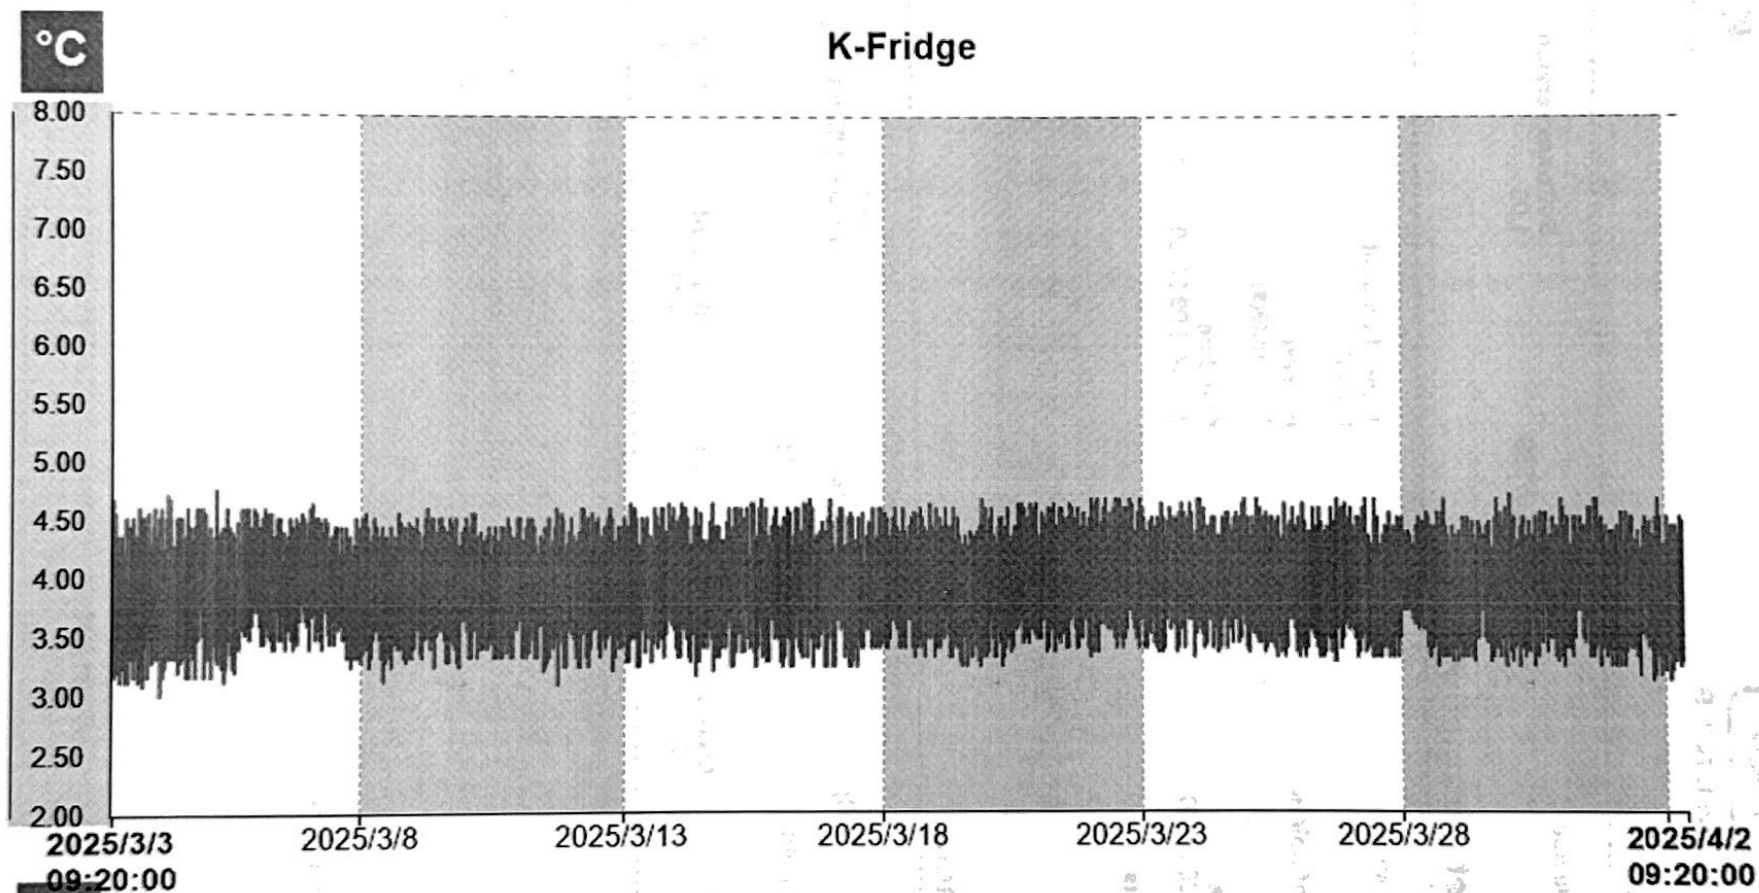



K-Fridge
2025/4/2 09:33:37

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07539] Ch-int1 K□□ [°C]	2881	3.0	4.8	3.97	0.41	3.98