

Chih-I Wu

02 Jun 2025



K-Fridge
2025/6/2 09:14:00

Device

Type of device	Serial n°	Software version
KH 50	OK 16.05.07539	1.06


Dataset parameters

Dataset name	Type of dataset
K-Fridge	Instant
Number of points	Interval
3072	15 minute(s)
Start date	End date
2025/5/1 09:25:00	2025/6/2 09:10:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 K□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.0	4.8	3.98
		Standard
		0.40
		MKT
		3.99

Peak A/T 80
2025-5-11

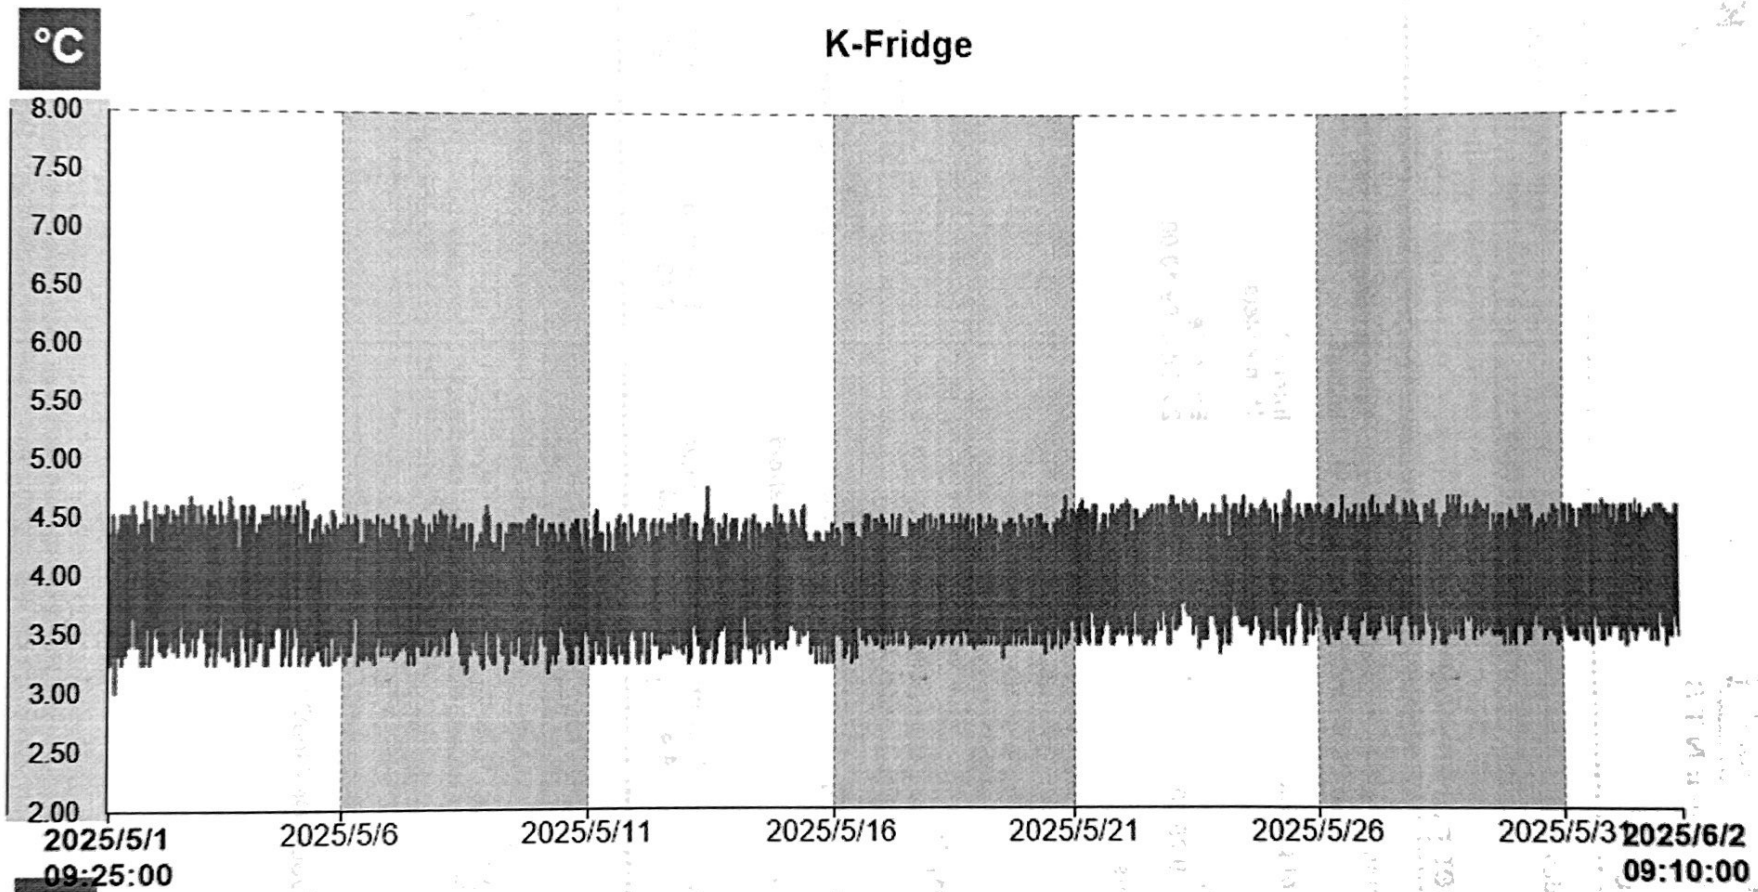

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07539]						
Ch-int1 K□□ [°C]	3072	3.0	4.8	3.98	0.40	3.99