

Chih-I Wu
01 Jul 2025



K-Fridge
2025/7/1 08:59:10

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07539	1.06

Dataset parameters

Dataset name	Type of dataset
K-Fridge	Instant
Number of points	Interval
2782	15 minute(s)
Start date	End date
2025/6/2 09:35:00	2025/7/1 08:50:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 K□□ [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
3.1	5.1	3.95	0.39	3.96

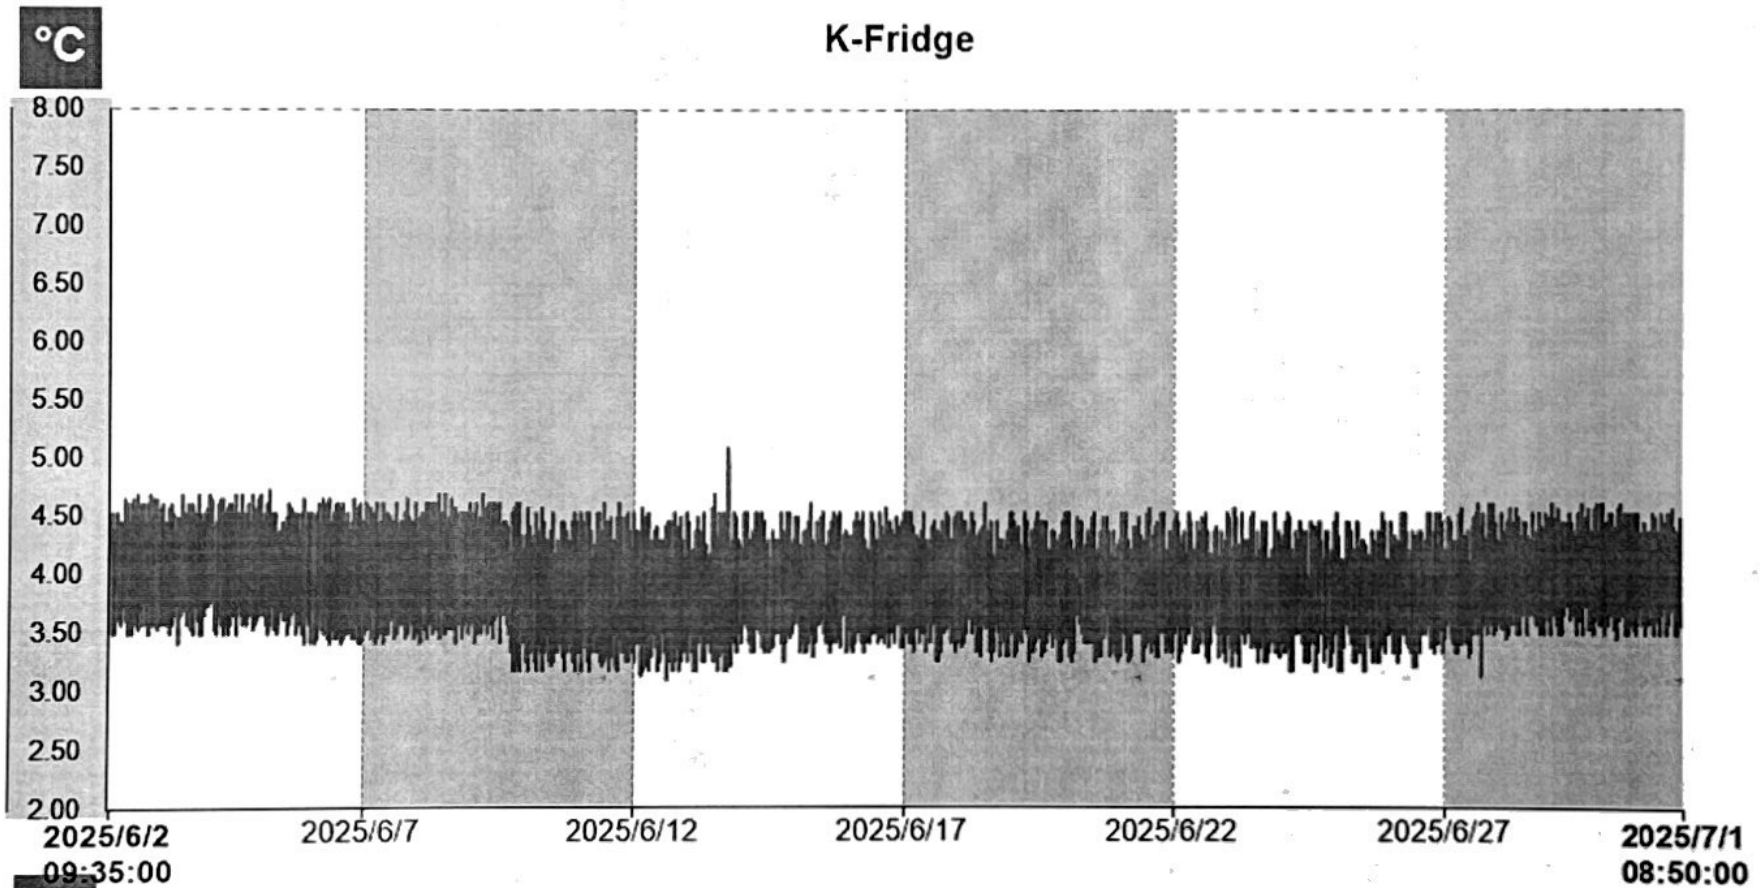

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07539]						
Ch-int1 KGD [°C]	2782	3.1	5.1	3.95	0.39	3.96