



K-Fridge back-up

2025/8/1 08:54:38

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07541	1.06

Dataset parameters

Dataset name	Type of dataset
K-Fridge back-up	Instant
Number of points	Interval
2978	15 minute(s)
Start date	End date
2025/7/1 08:35:00	2025/8/1 08:50:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 K-Fridge [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
2.9	5.5	3.93
		Standard
		0.36
		MKT
		3.94

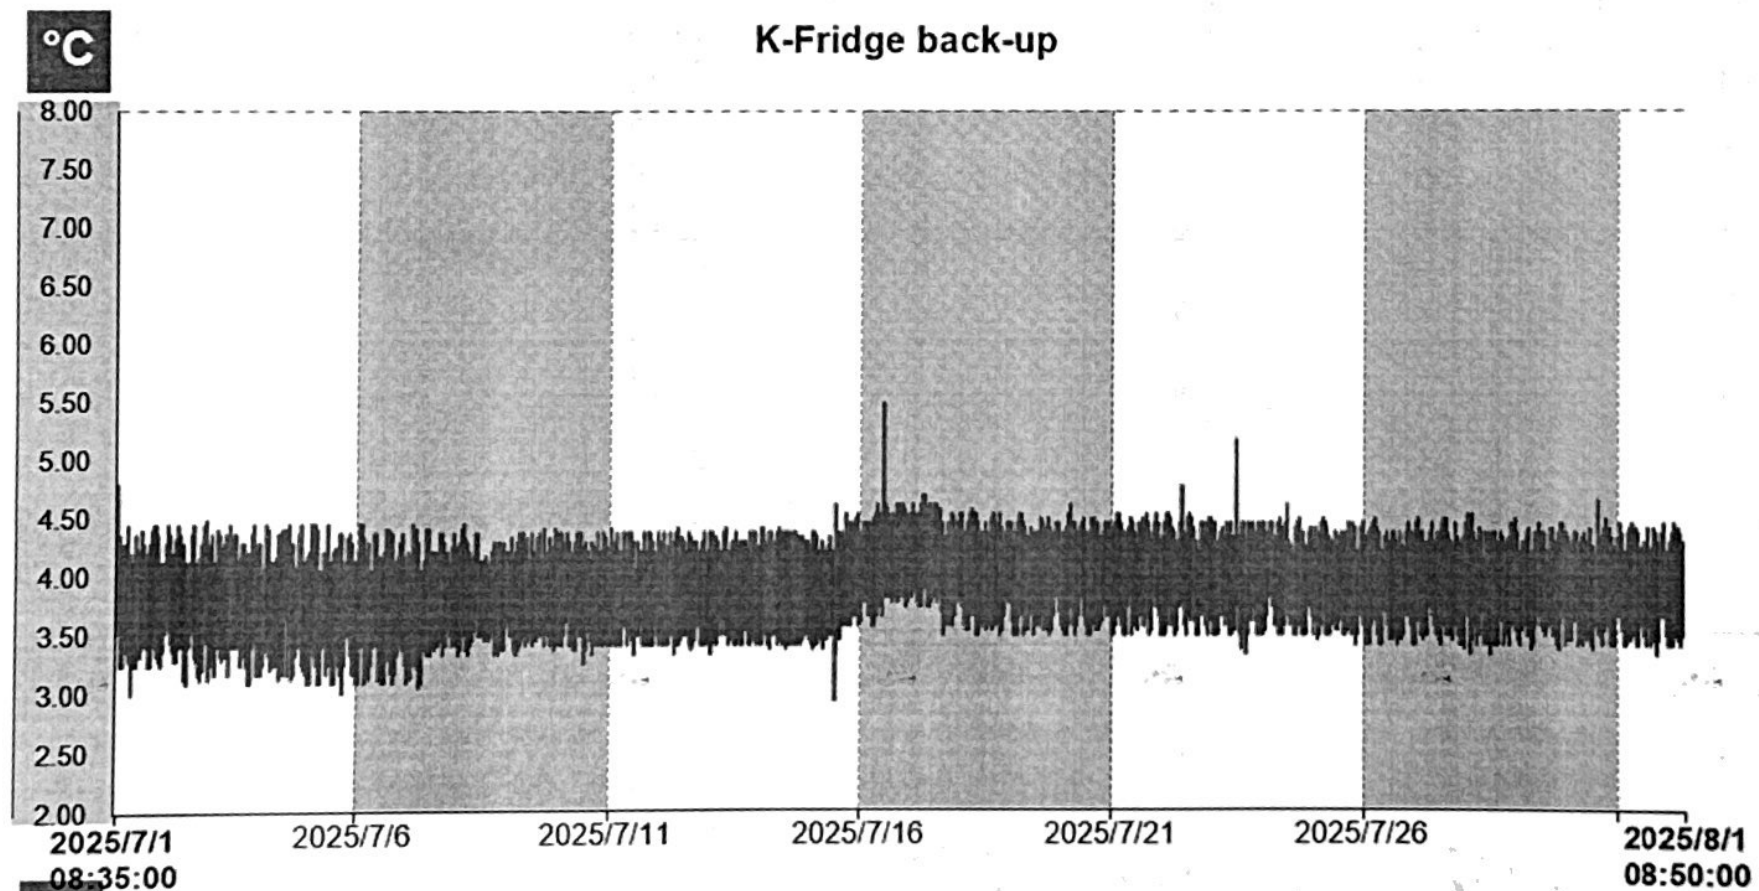



K-Fridge back-up

2025/8/1 08:54:38

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07541]						
Ch-int1 K-Fridge [°C]	2978	2.9	5.5	3.93	0.36	3.94