



K-Fridge
2025/9/1 09:14:32

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07539	1.06

Dataset parameters

Dataset name	Type of dataset
K-Fridge	Instant
Number of points	Interval
4321	15 minute(s)
Start date	End date
2025/7/18 09:00:00	2025/9/1 09:00:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 K□□ [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
2.9	4.7	3.89	0.39	3.90

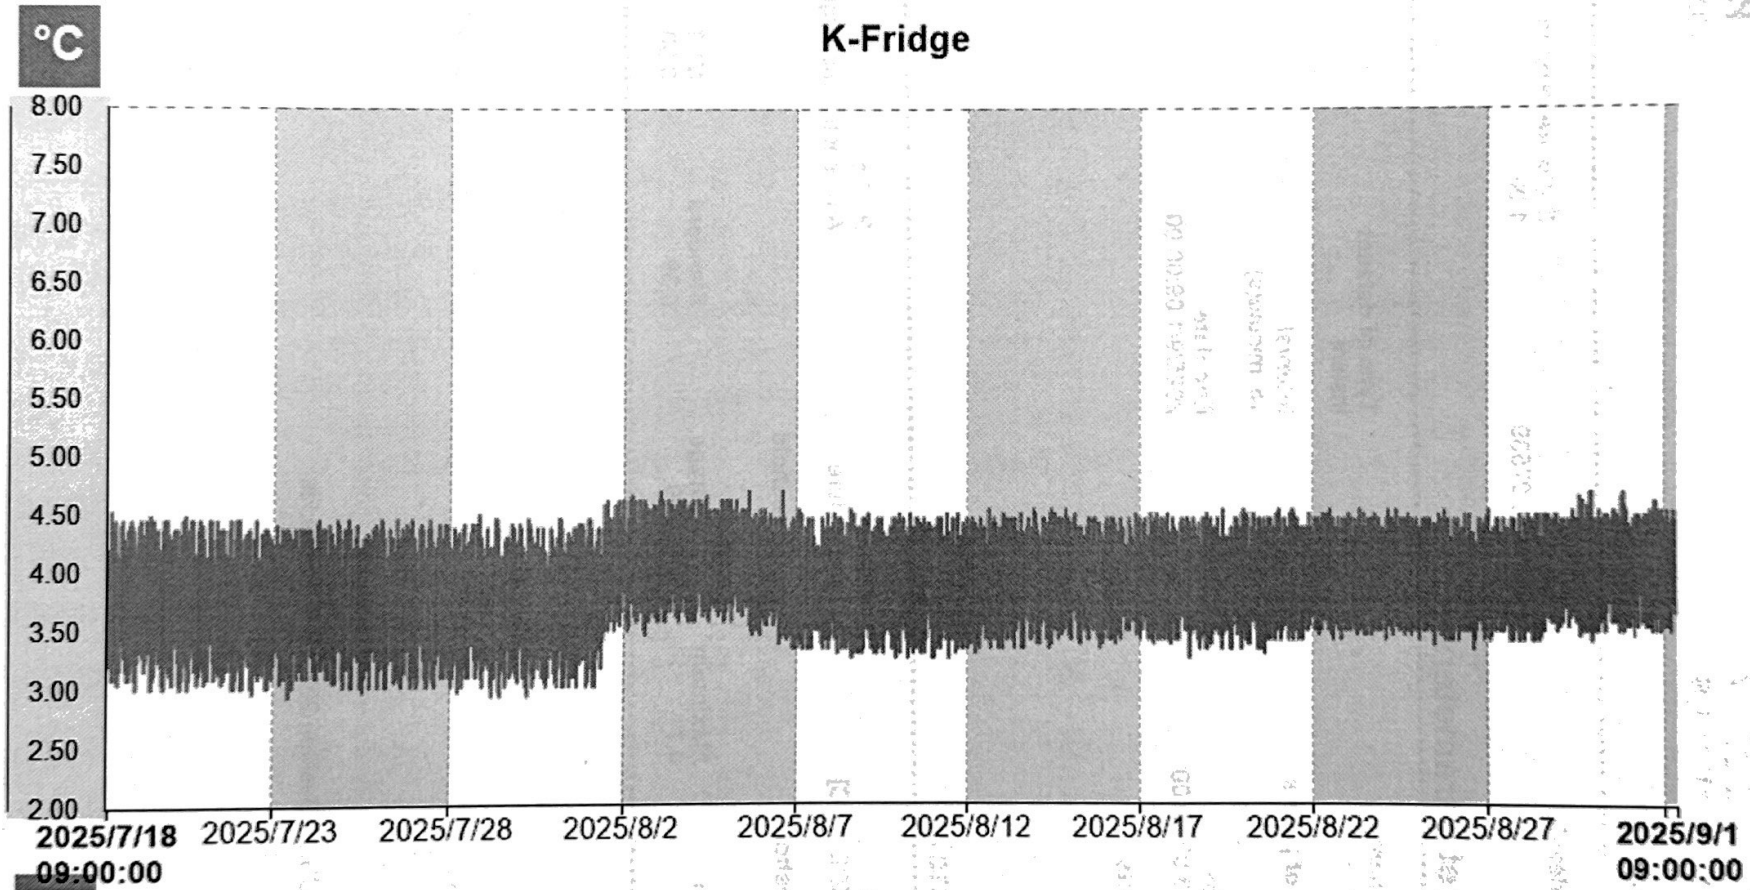



K-Fridge
2025/9/1 09:14:32

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07539] Ch-int1 K [°C]	4321	2.9	4.7	3.89	0.39	3.90