

Chih-I Wu

03 Nov 2025



K-Fridge
2025/11/3 10:26:38

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07539	1.06

Dataset parameters

Dataset name	Type of dataset
K-Fridge	Instant
Number of points	Interval
6051	15 minute(s)
Start date	End date
2025/9/1 09:50:00	2025/11/3 10:20:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 K□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.2	4.7	3.94
		Standard
		0.35
		MKT
		3.95

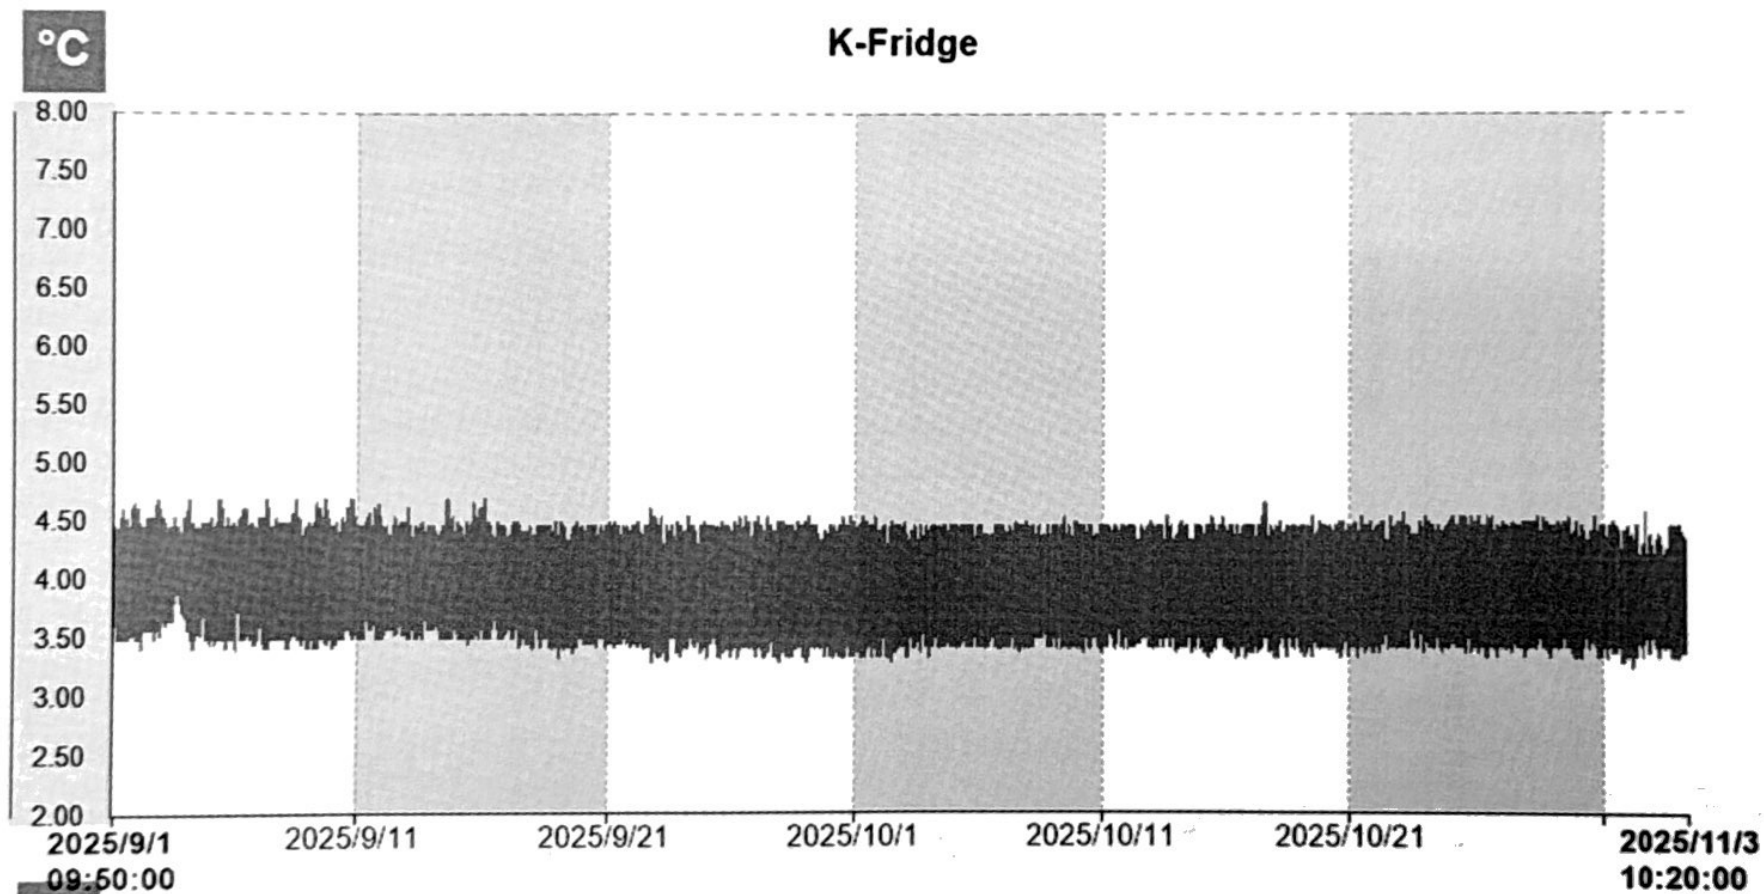

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07539]						
Ch-int1 K [°C]	6051	3.2	4.7	3.94	0.35	3.95