



## K-Fridge back-up

2025/12/1 09:51:49

### Device

---

Type of device	Serial n°	Software version
KH 50	OK 16.05.07541	1.06

### Dataset parameters

---


Dataset name	Type of dataset
K-Fridge back-up	Instant
Number of points	Interval
5856	15 minute(s)
Start date	End date
2025/10/1 10:00:00	2025/12/1 09:45:00
Comments	

### Channels

---

Channel	Measure	Probe		
Ch-int1 K-Fridge [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
3.2	5.5	3.92	0.34	3.93

---

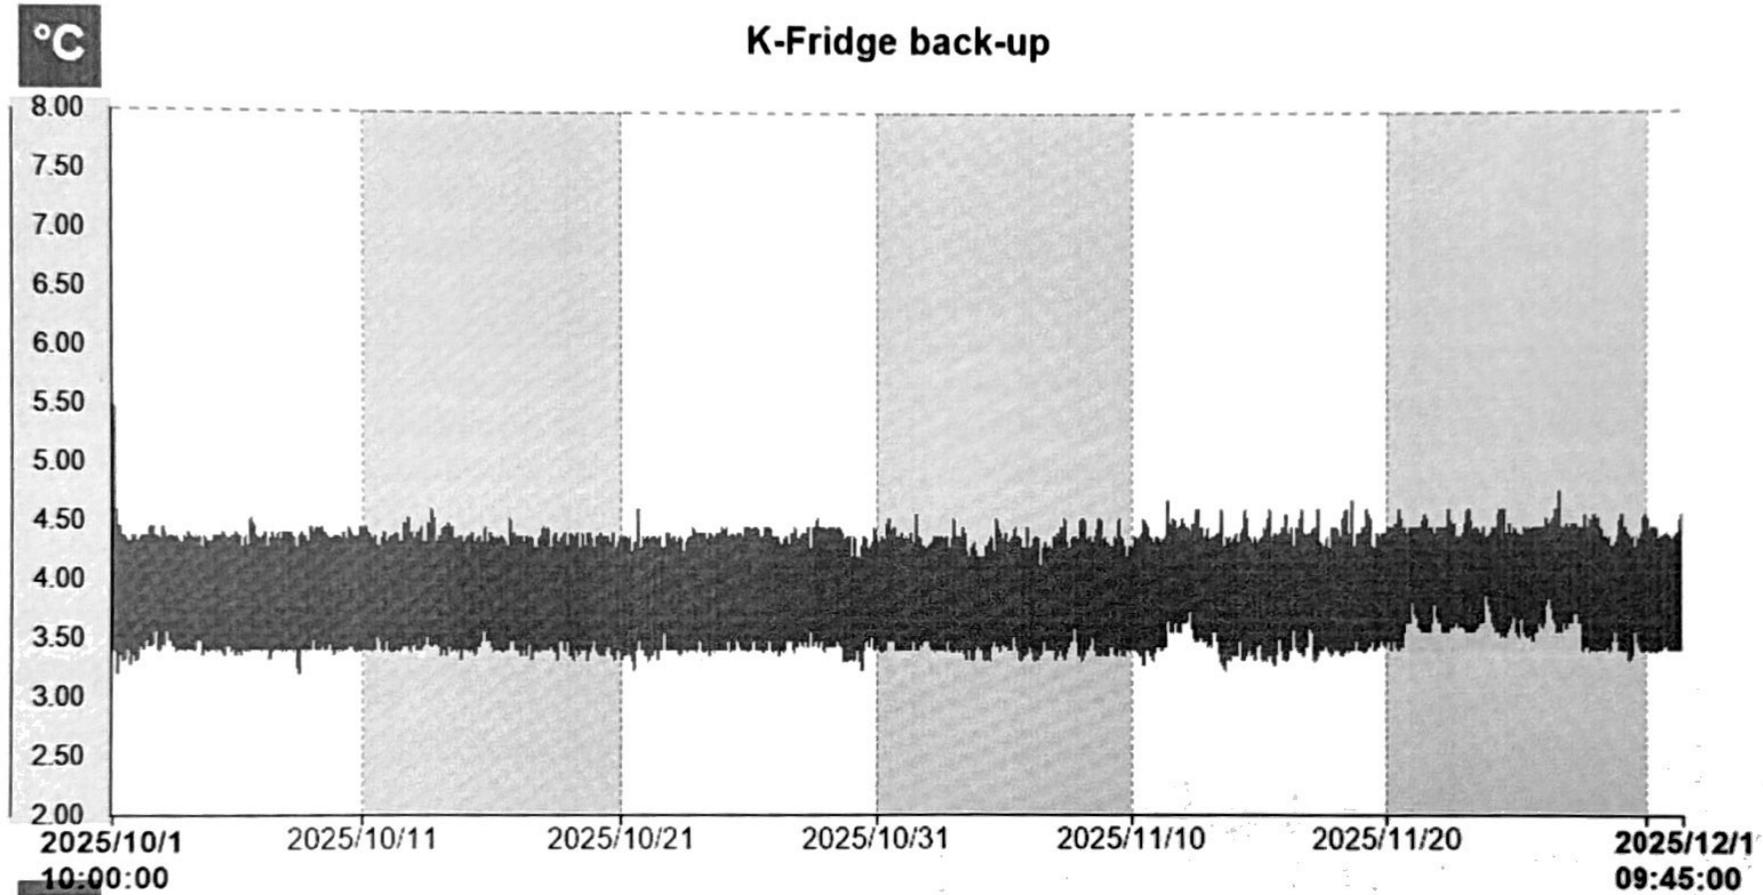



# K-Fridge back-up

2025/12/1 09:51:49

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
<b>KH.50 [OK 16.05.07541]</b> Ch-int1 K-Fridge [°C]	5856	3.2	5.5	3.92	0.34	3.93