



K-Fridge
2026/3/2 09:44:43

Device


Type of device KH 50	Serial n° OK 16.05.07539	Software version 1.06
-------------------------	-----------------------------	--------------------------

Dataset parameters

Dataset name K-Fridge	Type of dataset Instant
Number of points 5657	Interval 15 minute(s)
Start date 2026/1/2 11:35:00	End date 2026/3/2 09:35:00
Comments	

Channels

Channel Ch-int1 K□□ [°C]	Measure Temperature	Probe Ambient thermo-hygro		
Low threshold 2.0	High threshold 8.0			
Minimum 3.2	Maximum 5.3	Average 3.96	Standard 0.35	MKT 3.97

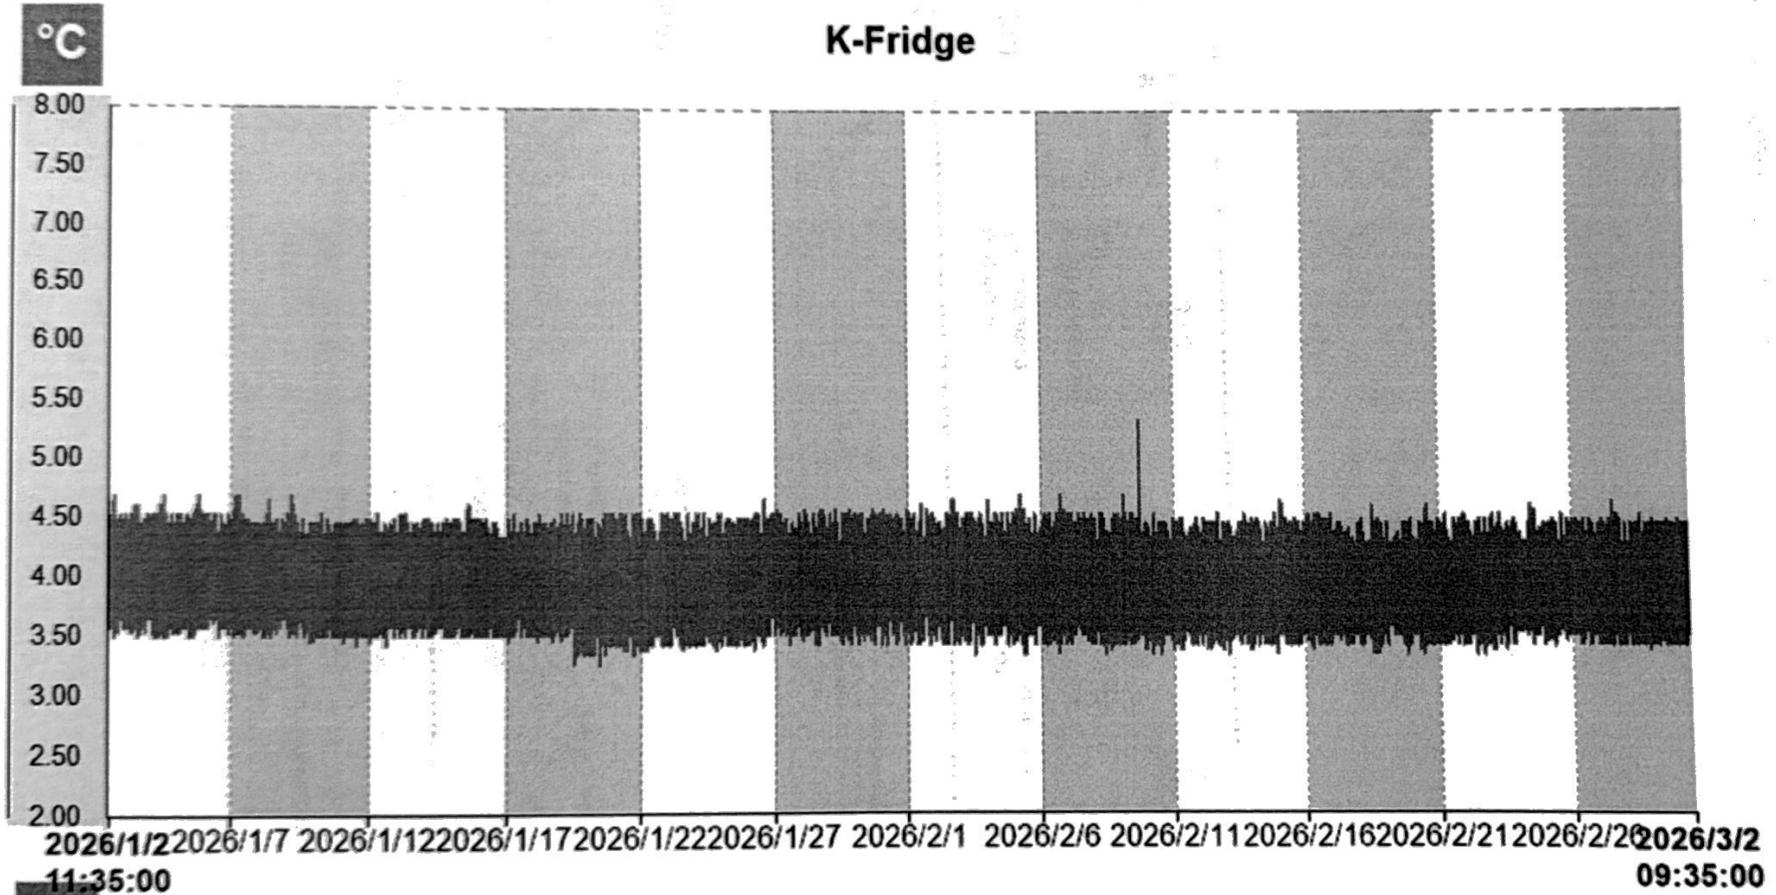

05:15:00
05:15:00



K-Fridge
2026/3/2 09:44:43

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK:16.05.07539] Ch-int1 K [°C]	5657	3.2	5.3	3.96	0.35	3.97