



K-Fridge
2024/4/1 10.01.17

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07539	1.06

Dataset parameters

Dataset name	Type of dataset
K-Fridge	Instant
Number of points	Interval
2975	15 minute(s)
Start date	End date
2024/3/1 10 20 00	2024/4/1 09 50 00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 K□□ [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
3.3	6.4	4.67	0.41	4.68

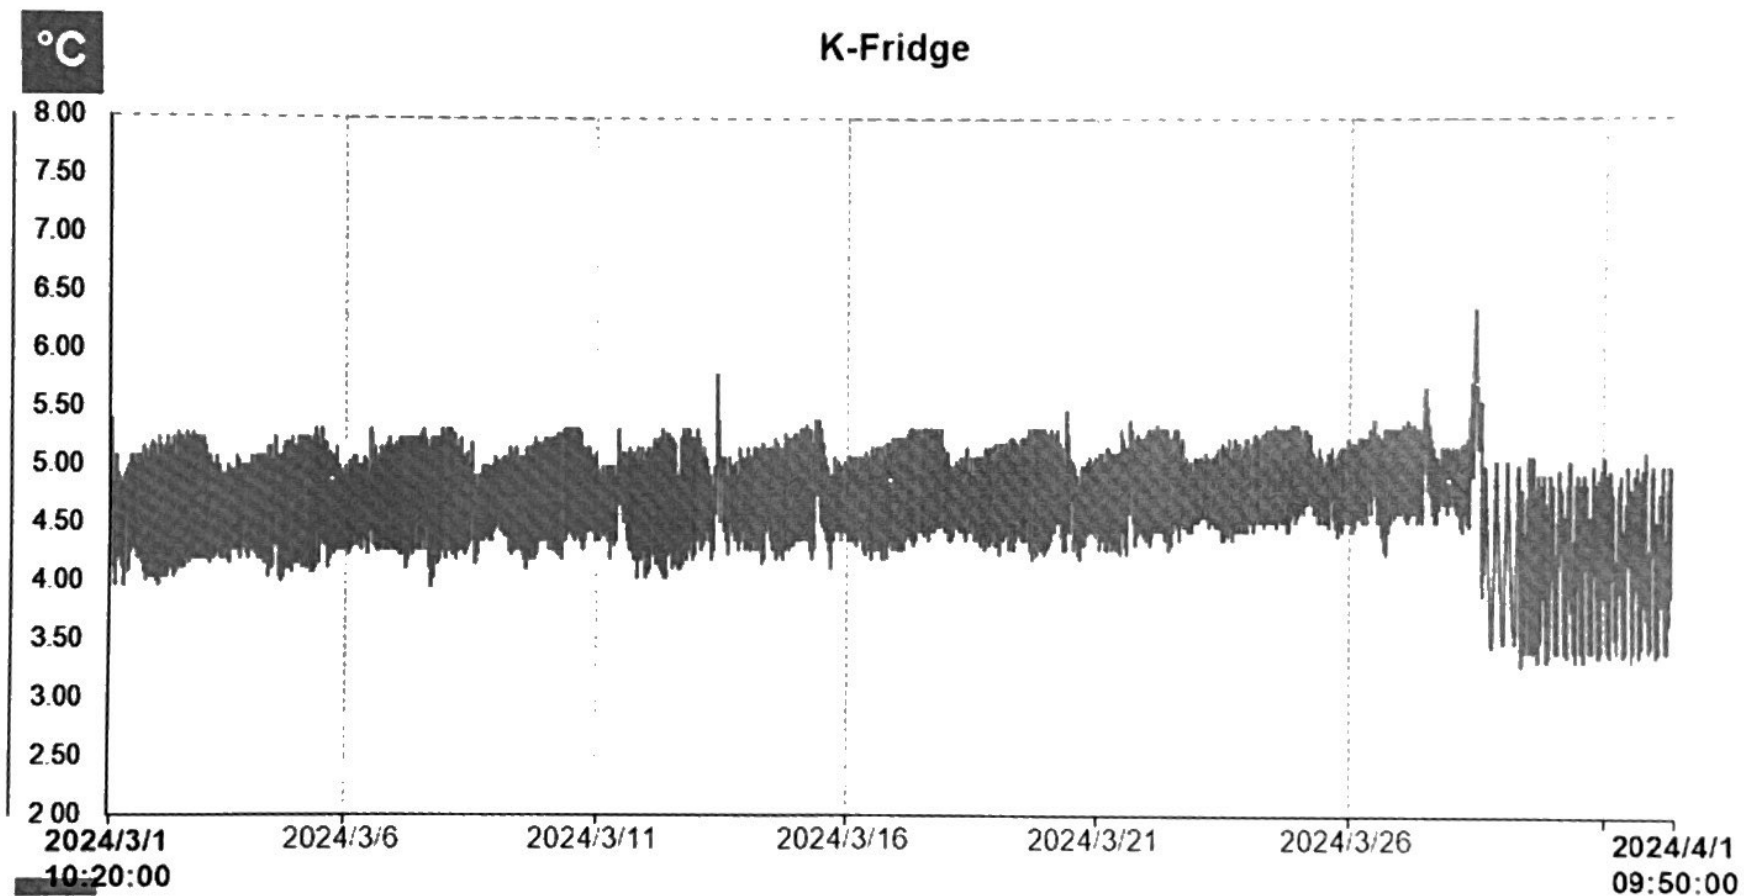



	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07539] Ch-int1 K [°C]	2975	3.3	6.4	4.67	0.41	4.68