



# K-Fridge back-up

2026/2/2 08:26:45

## Device

Type of device	Serial n°	Software version
KH 50	OK 16.05.07541	1.06


## Dataset parameters

Dataset name	Type of dataset
K-Fridge back-up	Instant
Number of points	Interval
6040	15 minute(s)
Start date	End date
2025/12/1 10:30:00	2026/2/2 08:15:00

## Comments

## Channels

Channel	Measure	Probe		
Ch-int1 K-Fridge [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
2.7	4.9	3.80	0.41	3.81

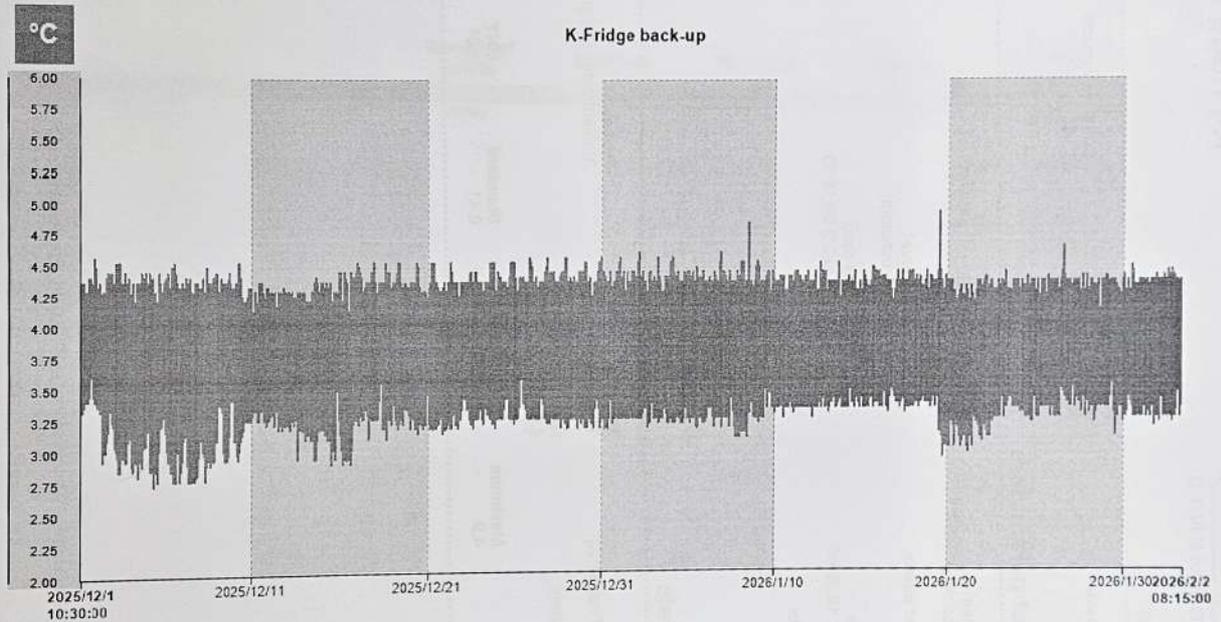



# K-Fridge back-up

2026/2/2 08:26:45

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
<b>KH 50 [OK 16.05.07541]</b> Ch-int1 K-Fridge [°C]	6040	2.7	4.9	3.80	0.41	3.81