

Chih-I Wu
01 May 2024



M-Fridge
2024/5/1 09:30:34

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07542	1.06

Dataset parameters

Dataset name	Type of dataset
M-Fridge	Instant
Number of points	Interval
2880	15 minute(s)
Start date	End date
2024/4/1 09:30:00	2024/5/1 09:15:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 M□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.5	6.1	4.46
		Standard
		0.42
		MKT
		4.47

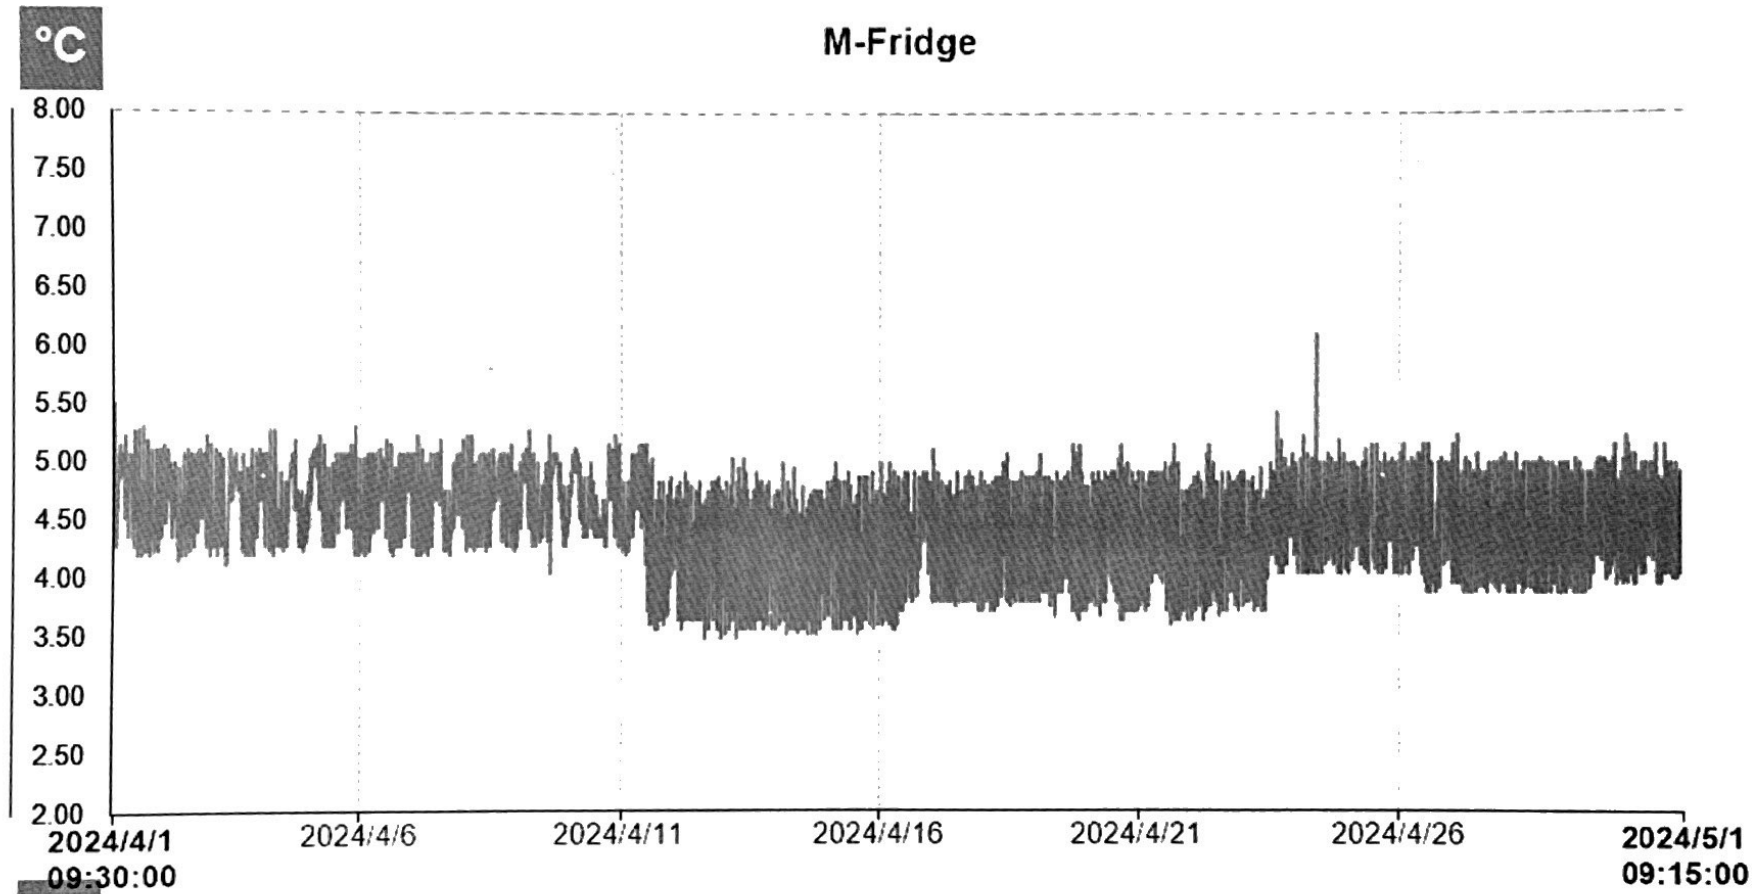



M-Fridge
2024/5/1 09:30:34

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07542] Ch-int1 M [°C]	2880	3.5	6.1	4.46	0.42	4.47