



M-Fridge
2024/6/3 08:58:11

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07542	1.06

Dataset parameters

Dataset name	Type of dataset
M-Fridge	Instant
Number of points	Interval
3165	15 minute(s)
Start date	End date
2024/5/1 09:50:00	2024/6/3 08:50:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 M□□ [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
3.8	5.5	4.70	0.32	4.71

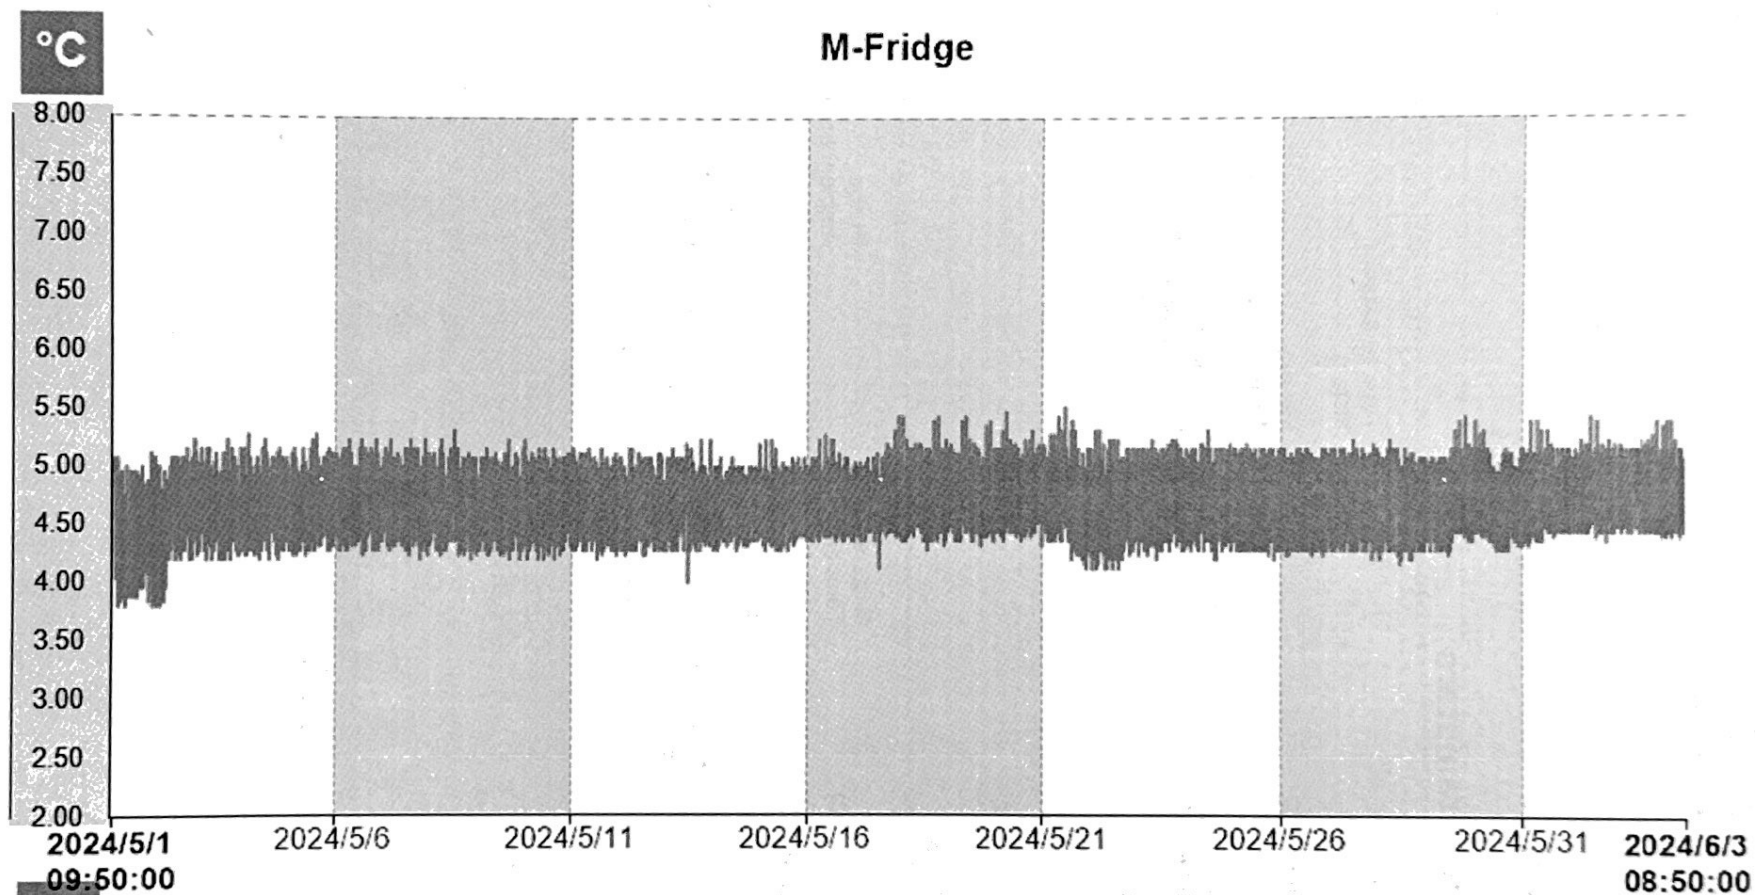



		Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07542]							
Ch-int1 M	[°C]	3165	3.8	5.5	4.70	0.32	4.71