

Chih-I Wu
01 Aug 2024



M-Fridge back up

2024/8/1 16:10:29

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07540	1.06

Dataset parameters

Dataset name	Type of dataset
M-Fridge back up	Instant
Number of points	Interval
2612	15 minute(s)
Start date	End date
2024/7/5 11:15:00	2024/8/1 16:00:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 M-Fridge [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
3.4	5.6	4.61	0.54	4.62

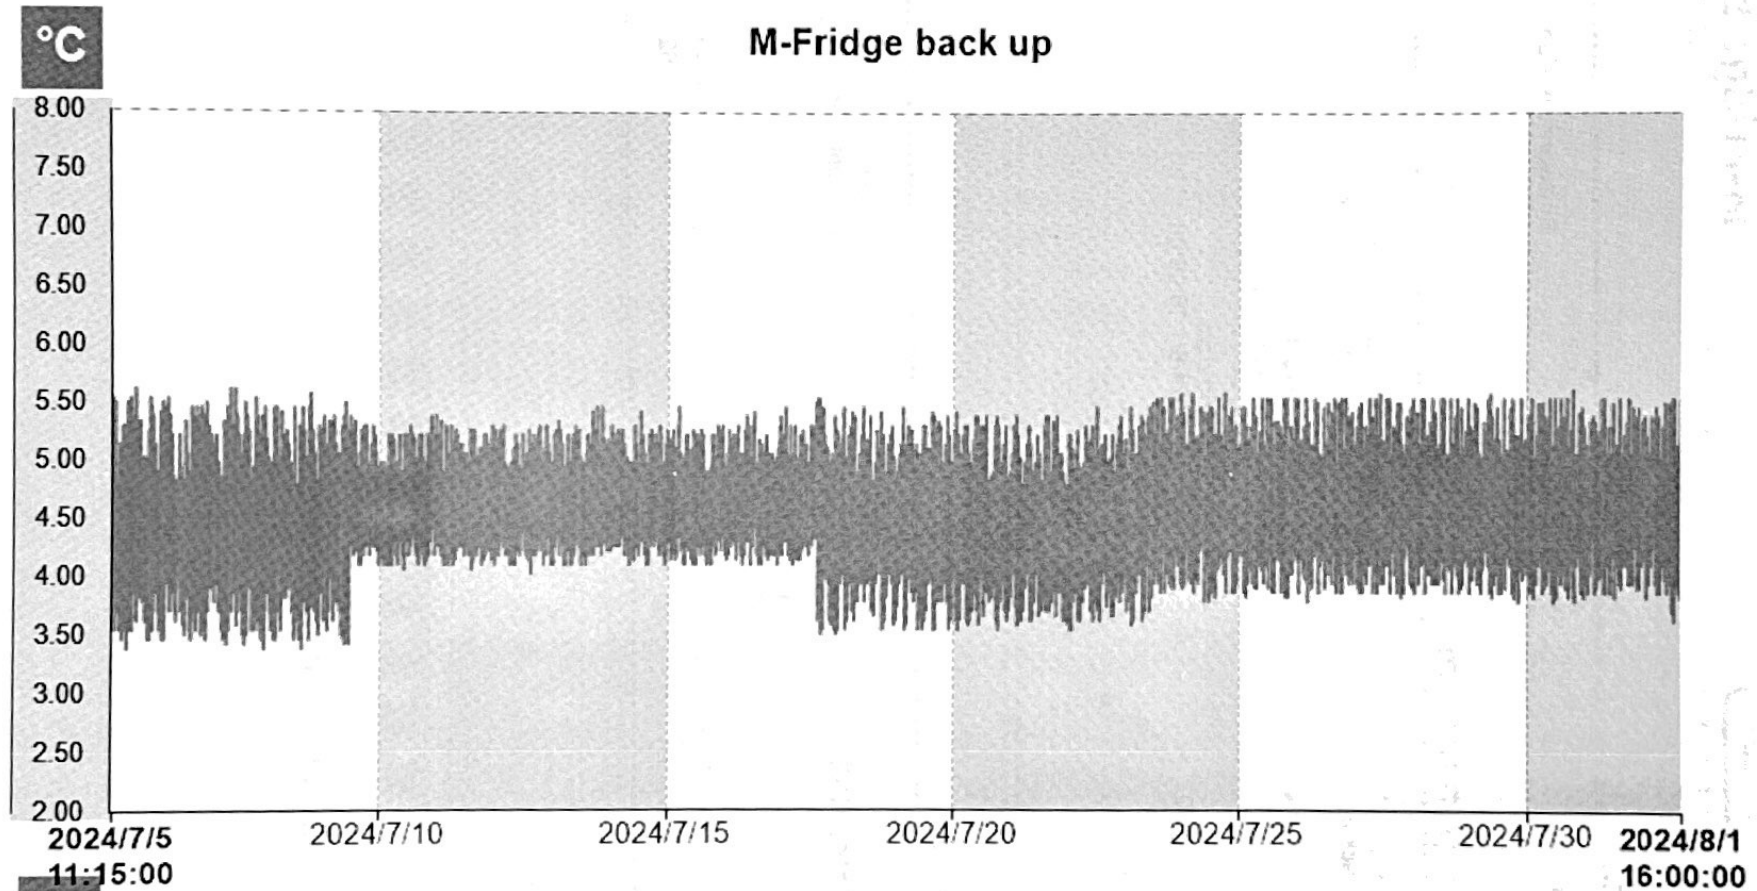



M-Fridge back up

2024/8/1 16:10:29

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07540] Ch-int1 M-Fridge [°C]	2612	3.4	5.6	4.61	0.54	4.62