



M-Fridge
2024/9/2 09:22:50

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07542	1.06

Dataset parameters

Dataset name	Type of dataset
M-Fridge	Instant
Number of points	Interval
3878	15 minute(s)
Start date	End date
2024/7/24 00:00:00	2024/9/2 09:15:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 M□□ [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
3.2	5.5	4.51	0.54	4.53

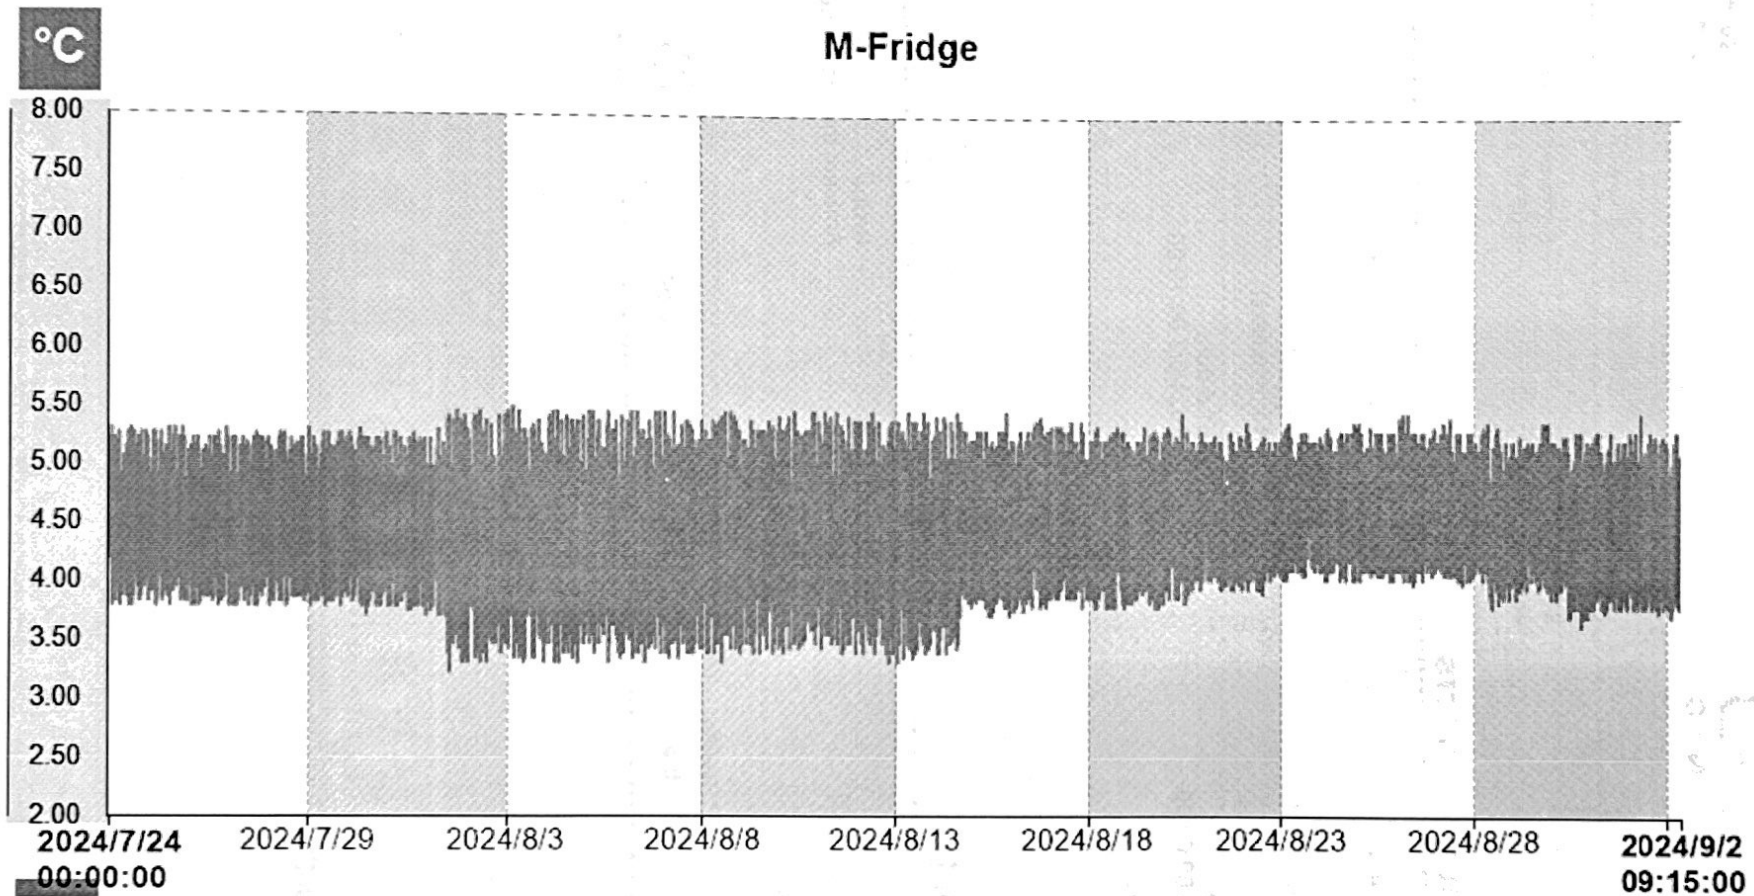



	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07542] Ch-int1 M [°C]	3878	3.2	5.5	4.51	0.54	4.53