



M-Fridge
2024/12/2 10:05:46

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07542	1.06

Dataset parameters

Dataset name	Type of dataset
M-Fridge	Instant
Number of points	Interval
2976	15 minute(s)
Start date	End date
2024/11/1 10:15:00	2024/12/2 10:00:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 M□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
2.9	6.0	4.33
		Standard
		0.69
		MKT
		4.36

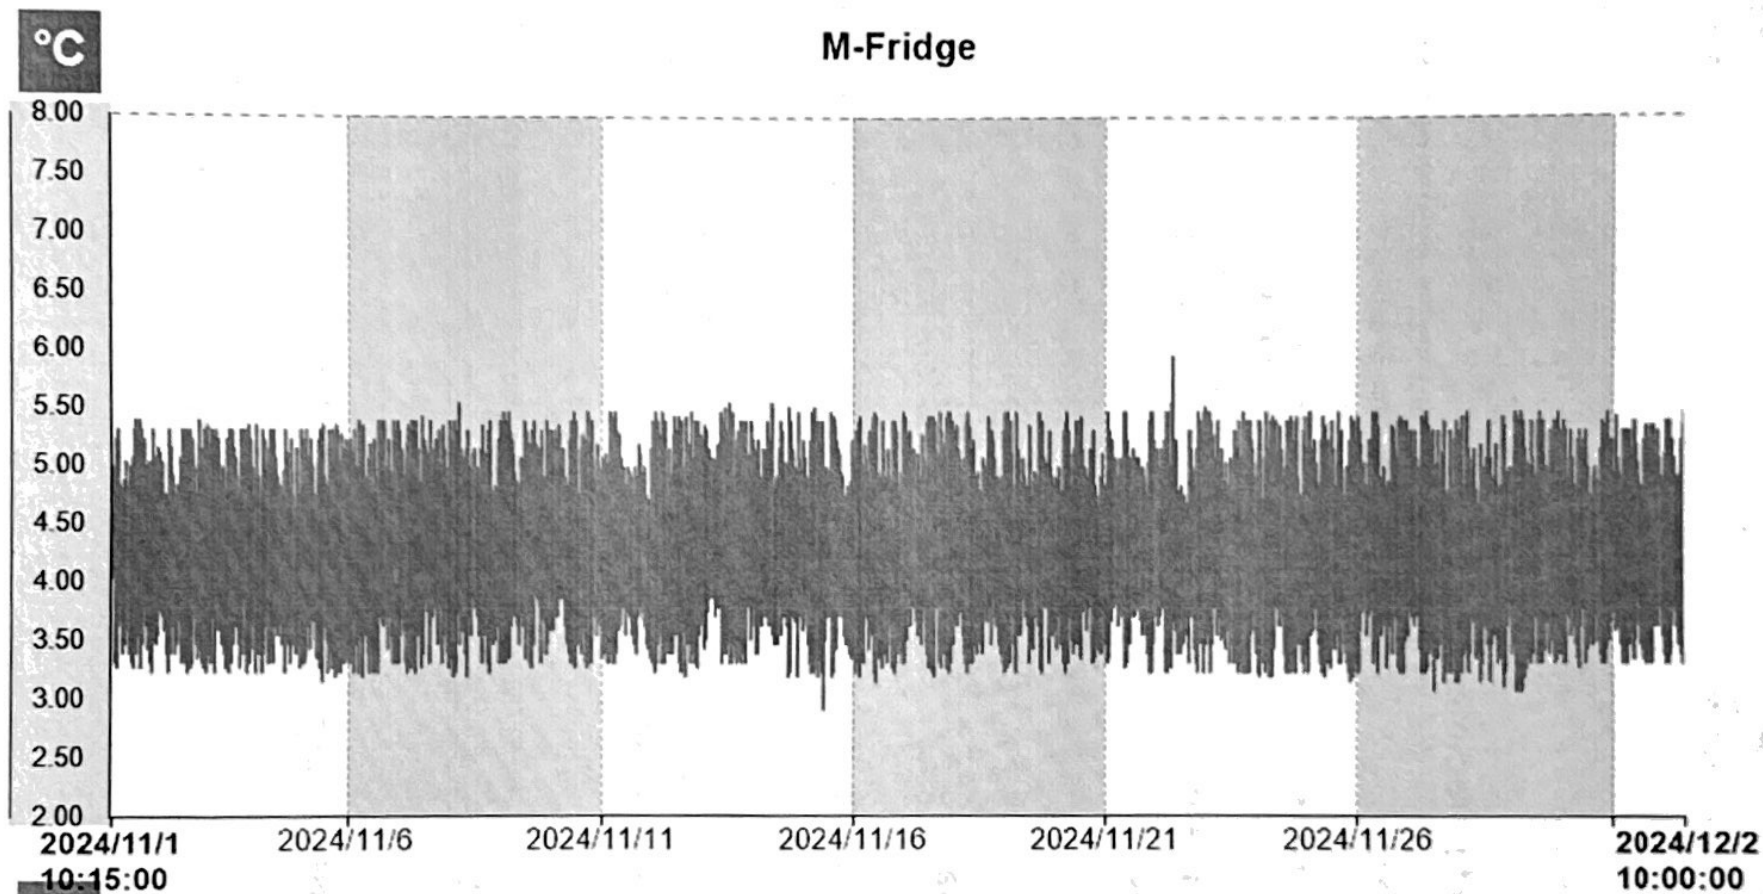



M-Fridge
2024/12/2 10:05:46

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07542] Ch-int1 M... [°C]	2976	2.9	6.0	4.33	0.69	4.36