

**M-Fridge**
2025/1/2 10:04:22**Device**


Type of device	Serial n°	Software version
KH 50	OK 16.05.07542	1.06

Dataset parameters

Dataset name	Type of dataset
M-Fridge	Instant
Number of points	Interval
2975	15 minute(s)
Start date	End date
2024/12/2 10:30:00	2025/1/2 10:00:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 M□□ [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
3.3	5.5	4.55	0.48	4.56

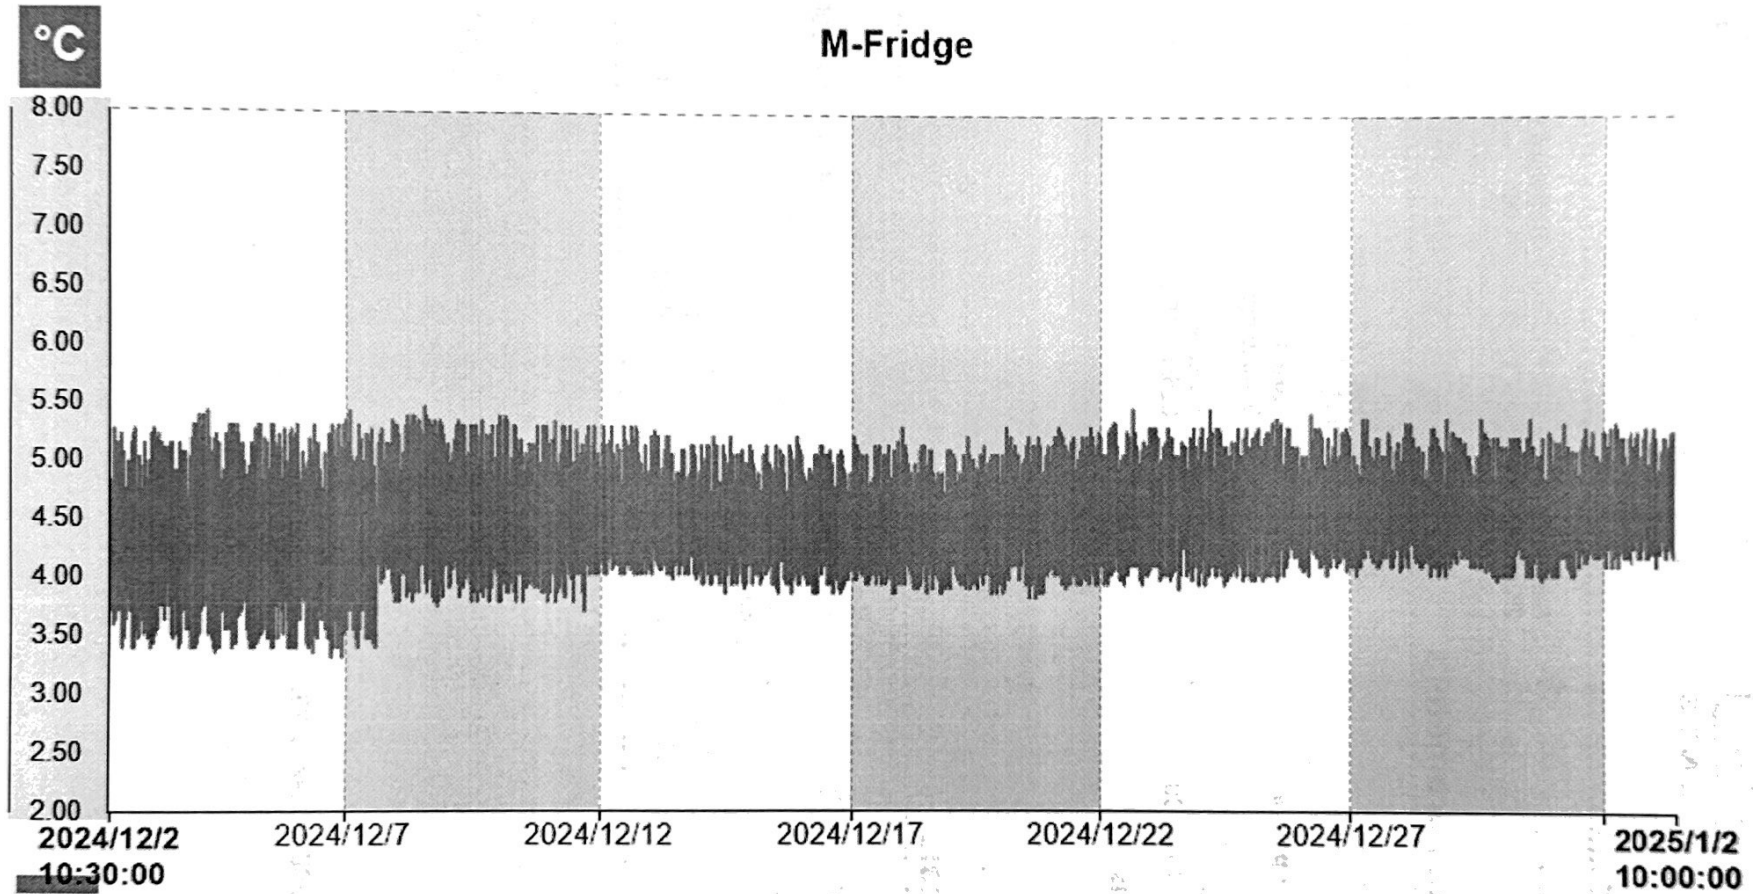



M-Fridge
2025/1/2 10:04:22

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07542] Ch-int1 M [°C]	2975	3.3	5.5	4.55	0.48	4.56