



M-Fridge
2025/3/3 09:35:18

Device

Type of device	Serial n°	Software version
KH 50	OK 16.05.07542	1.06


Dataset parameters

Dataset name	Type of dataset
M-Fridge	Instant
Number of points	Interval
2681	15 minute(s)
Start date	End date
2025/2/3 11:00:00	2025/3/3 09:00:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 M□□ [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
3.0	5.9	4.21	0.55	4.23

2025/3/3 09:35:18
M-Fridge

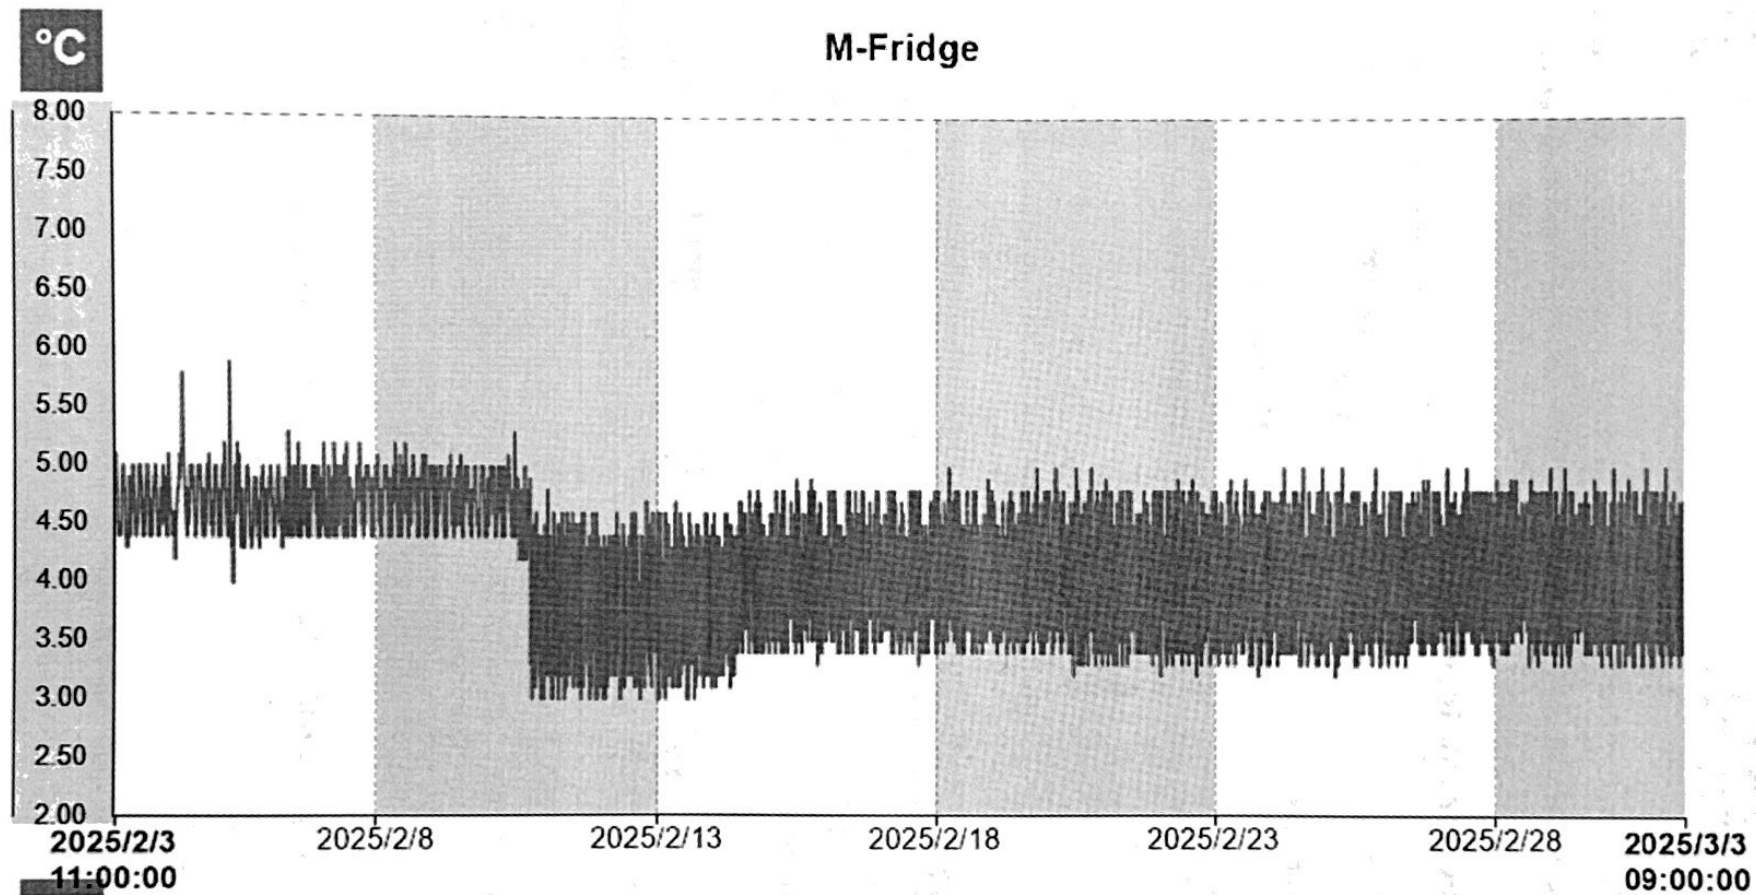

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07542] Ch-int1 M [°C]	2681	3.0	5.9	4.21	0.55	4.23