

Chih-I Wu
02 Apr 2025



M-Fridge
2025/4/2 09:58:48

Device


Type of device	Serial n°	Software version
KH 50	0K 16.05.07542	1.06

Dataset parameters

Dataset name	Type of dataset
M-Fridge	Instant
Number of points	Interval
2882	15 minute(s)
Start date	End date
2025/3/3 09:30:00	2025/4/2 09:45:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 M□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.1	5.1	4.09
		Standard
		0.49
		MKT
		4.11

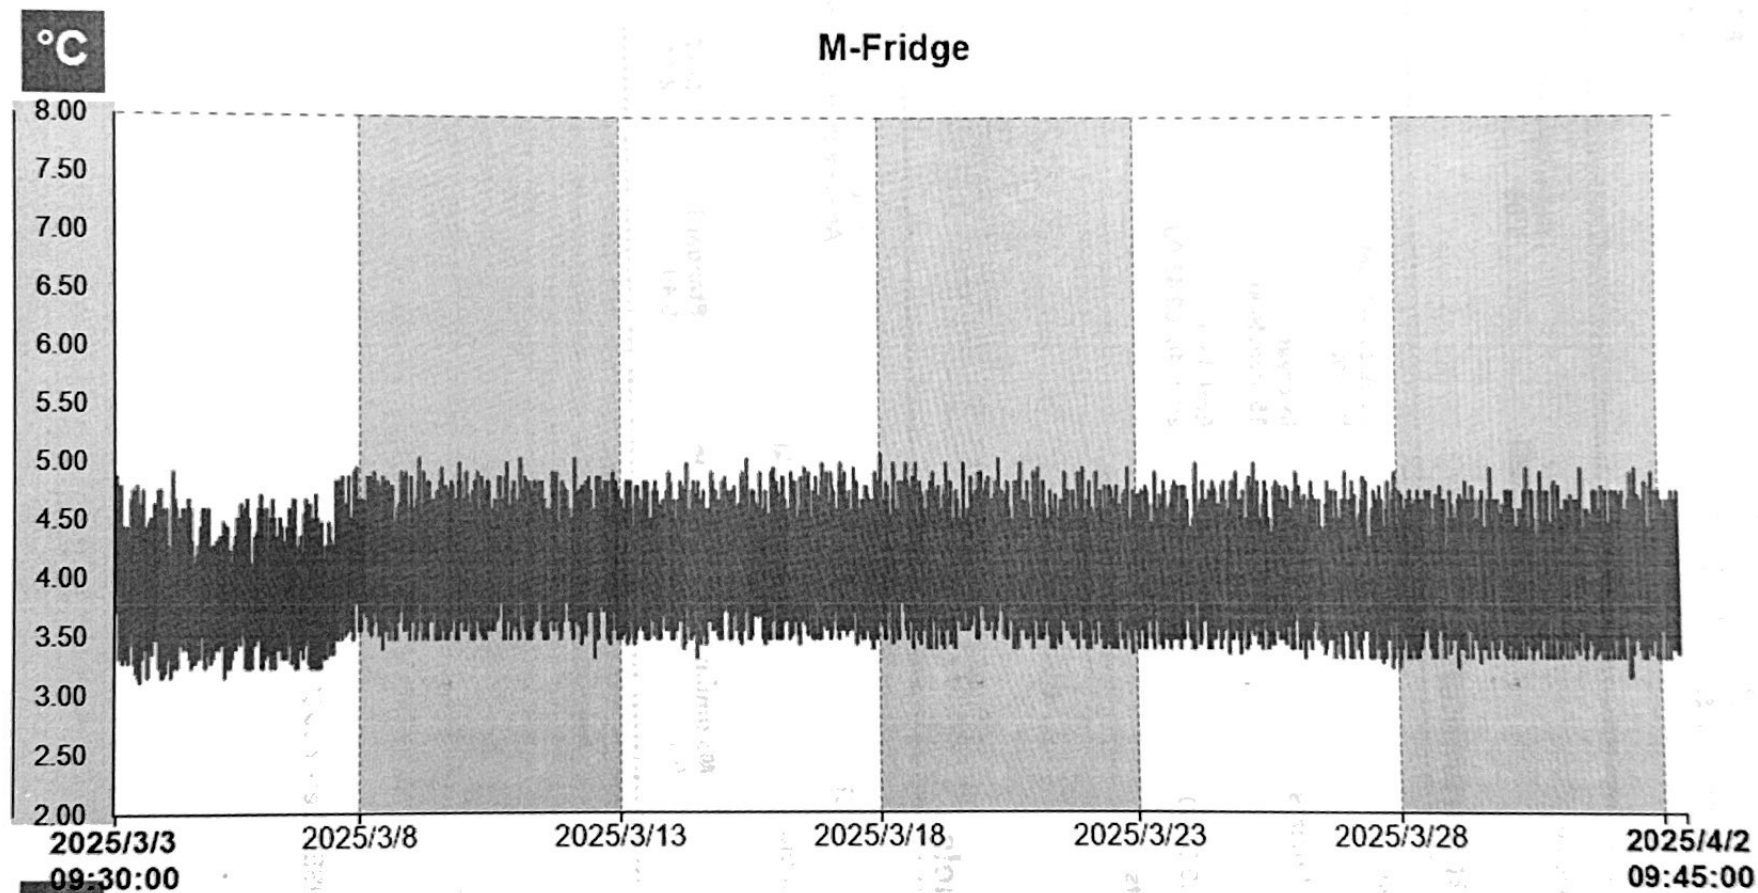



M-Fridge
2025/4/2 09:58:48

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07542] Ch-int1 M□□ [°C]	2882	3.1	5.1	4.09	0.49	4.11