


**M-Fridge**

2025/5/1 09:07:39

DeviceType of device
KH 50Serial n°
OK 16.05.07542Software version
1.06**Dataset parameters**Dataset name
M-FridgeType of dataset
InstantNumber of points
2780Interval
15 minute(s)Start date
2025/4/2 10:15:00End date
2025/5/1 09:00:00

Comments

ChannelsChannel
Ch-int1 M□□ [°C]Measure
TemperatureProbe
Ambient thermo-hygroLow threshold
2.0High threshold
8.0Minimum
3.2Maximum
5.1Average
4.06Standard
0.49MKT
4.07

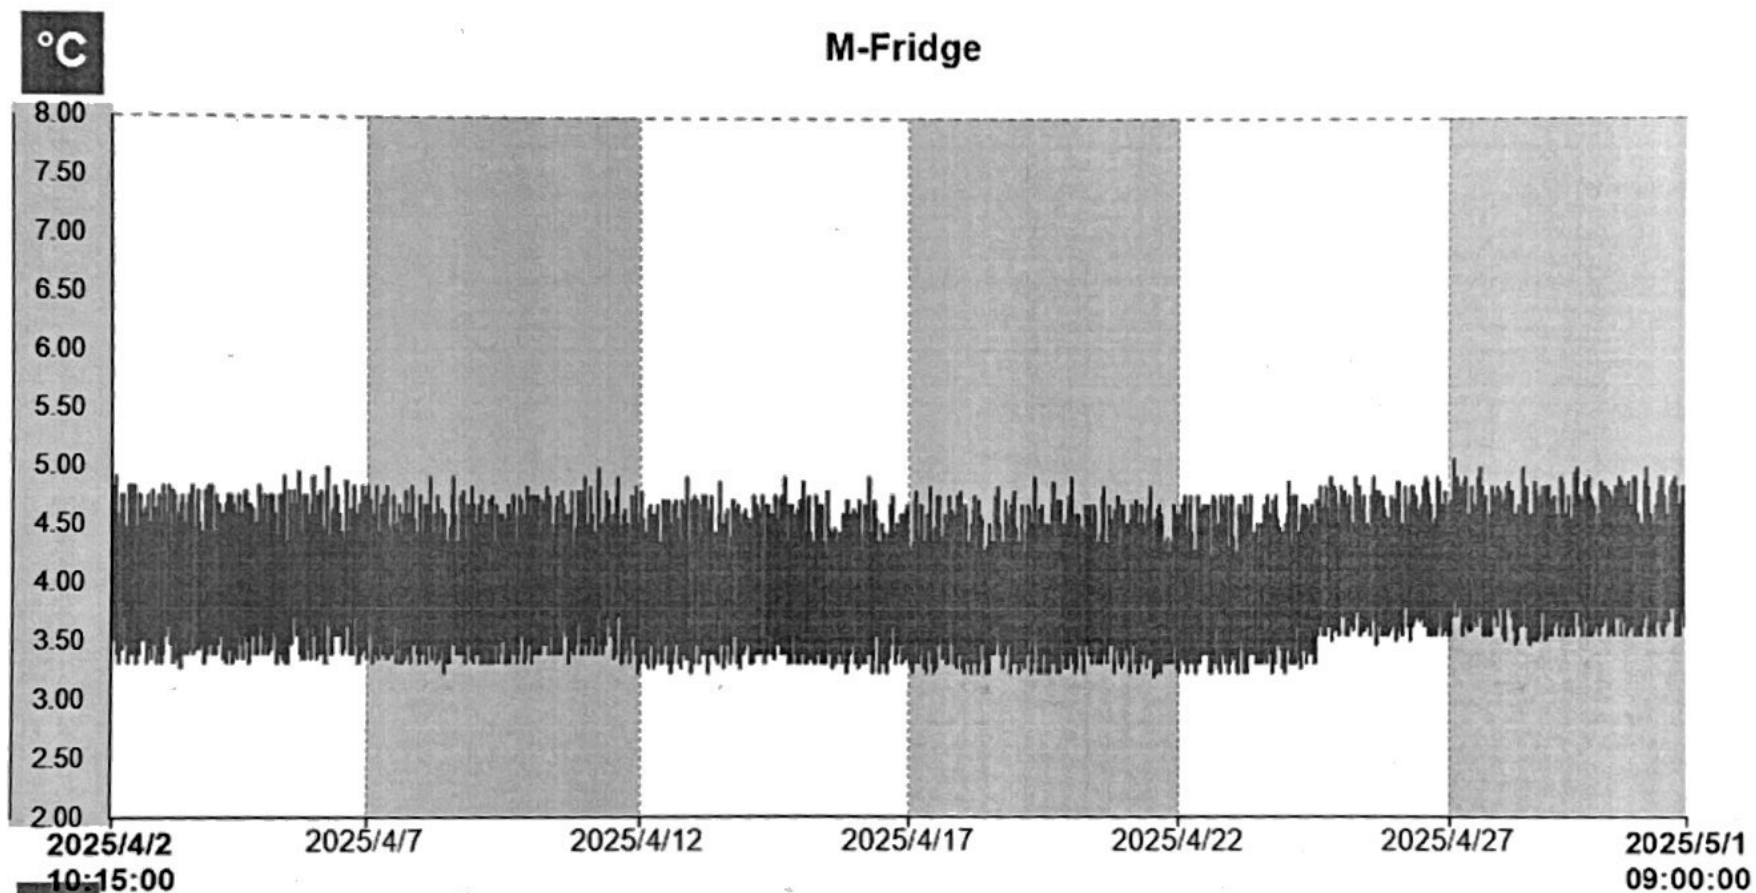

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [0K 16.05.07542]						
Ch-int1 M... [°C]	2780	3.2	5.1	4.06	0.49	4.07