

Chih-I Wu

02 Jun 2025



M-Fridge
2025/6/2 09:20:57

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07542	1.06

Dataset parameters

Dataset name	Type of dataset
M-Fridge	Instant
Number of points	Interval
3072	15 minute(s)
Start date	End date
2025/5/1 09:30:00	2025/6/2 09:15:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 M□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.2	5.2	4.20
		Standard
		0.47
		MKT
		4.22

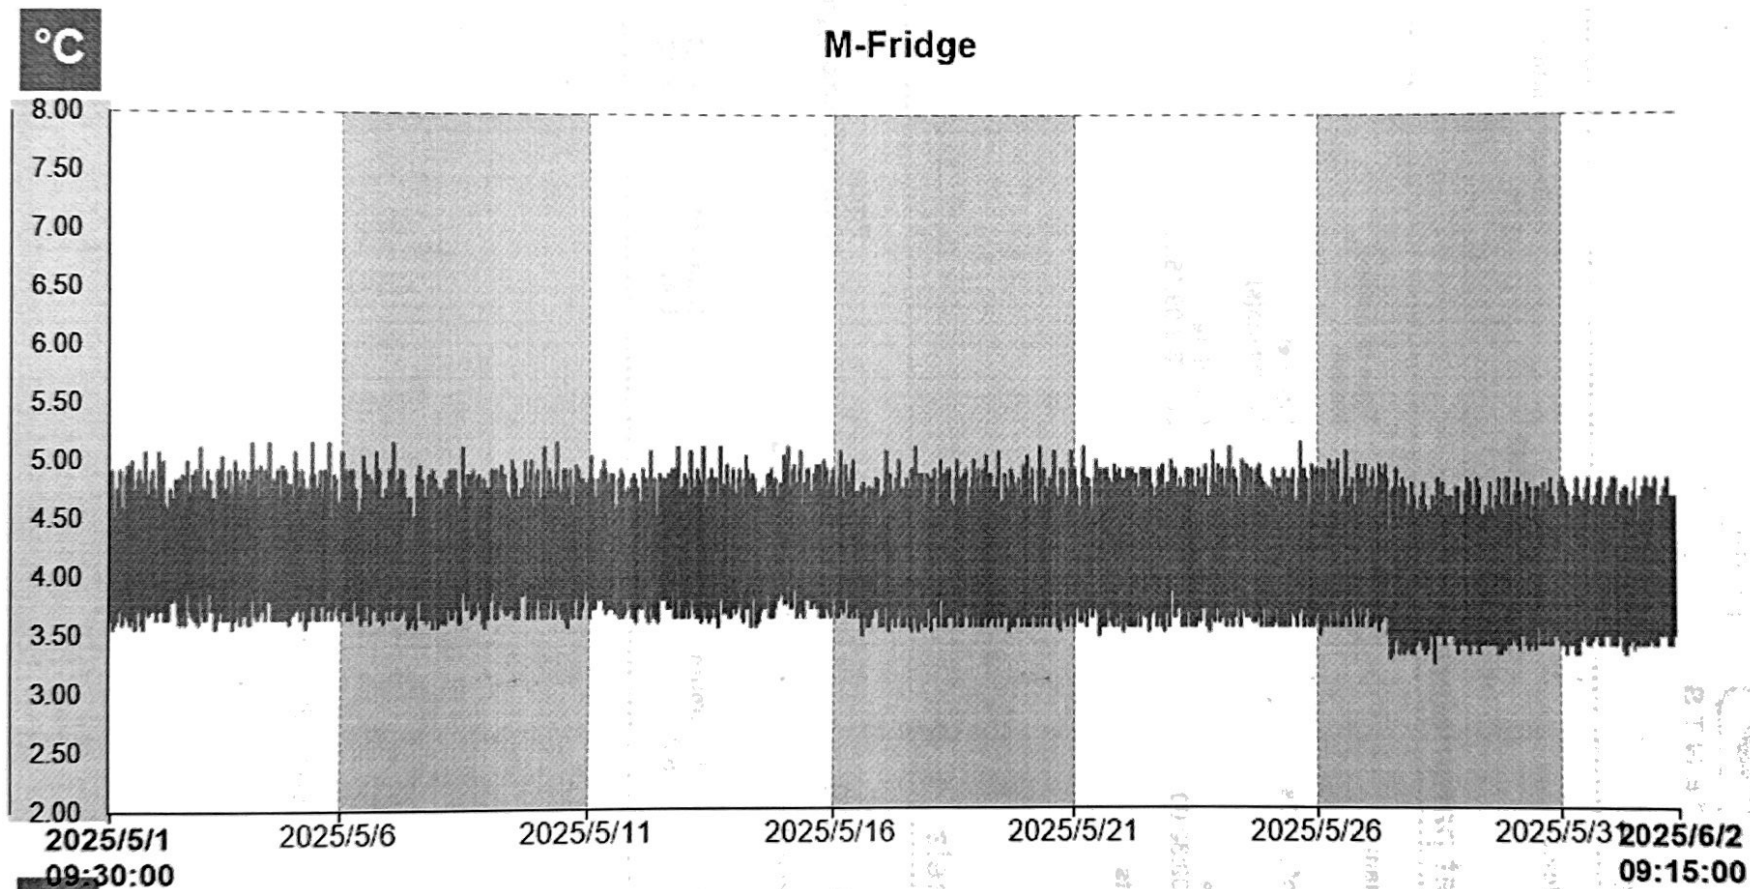

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [0K 16.05.07542]						
Ch-int1 M□□ [°C]	3072	3.2	5.2	4.20	0.47	4.22