

Chih-I Wu

01 Jul 2025



M-Fridge

2025/7/1 09:04:33

Device

Type of device
KH 50

Serial n°
0K 16.05.07542

Software version
1.06

Dataset parameters

Dataset name
M-Fridge

Type of dataset
Instant

Number of points
2782

Interval
15 minute(s)

Start date
2025/6/2 09:45:00

End date
2025/7/1 09:00:00

Comments

Channels

Channel
Ch-int1 M□□ [°C]

Measure
Temperature

Probe
Ambient thermo-hygro

Low threshold
2.0

High threshold
8.0


Minimum
3.1

Maximum
5.1

Average
4.09

Standard
0.49

MKT
4.11

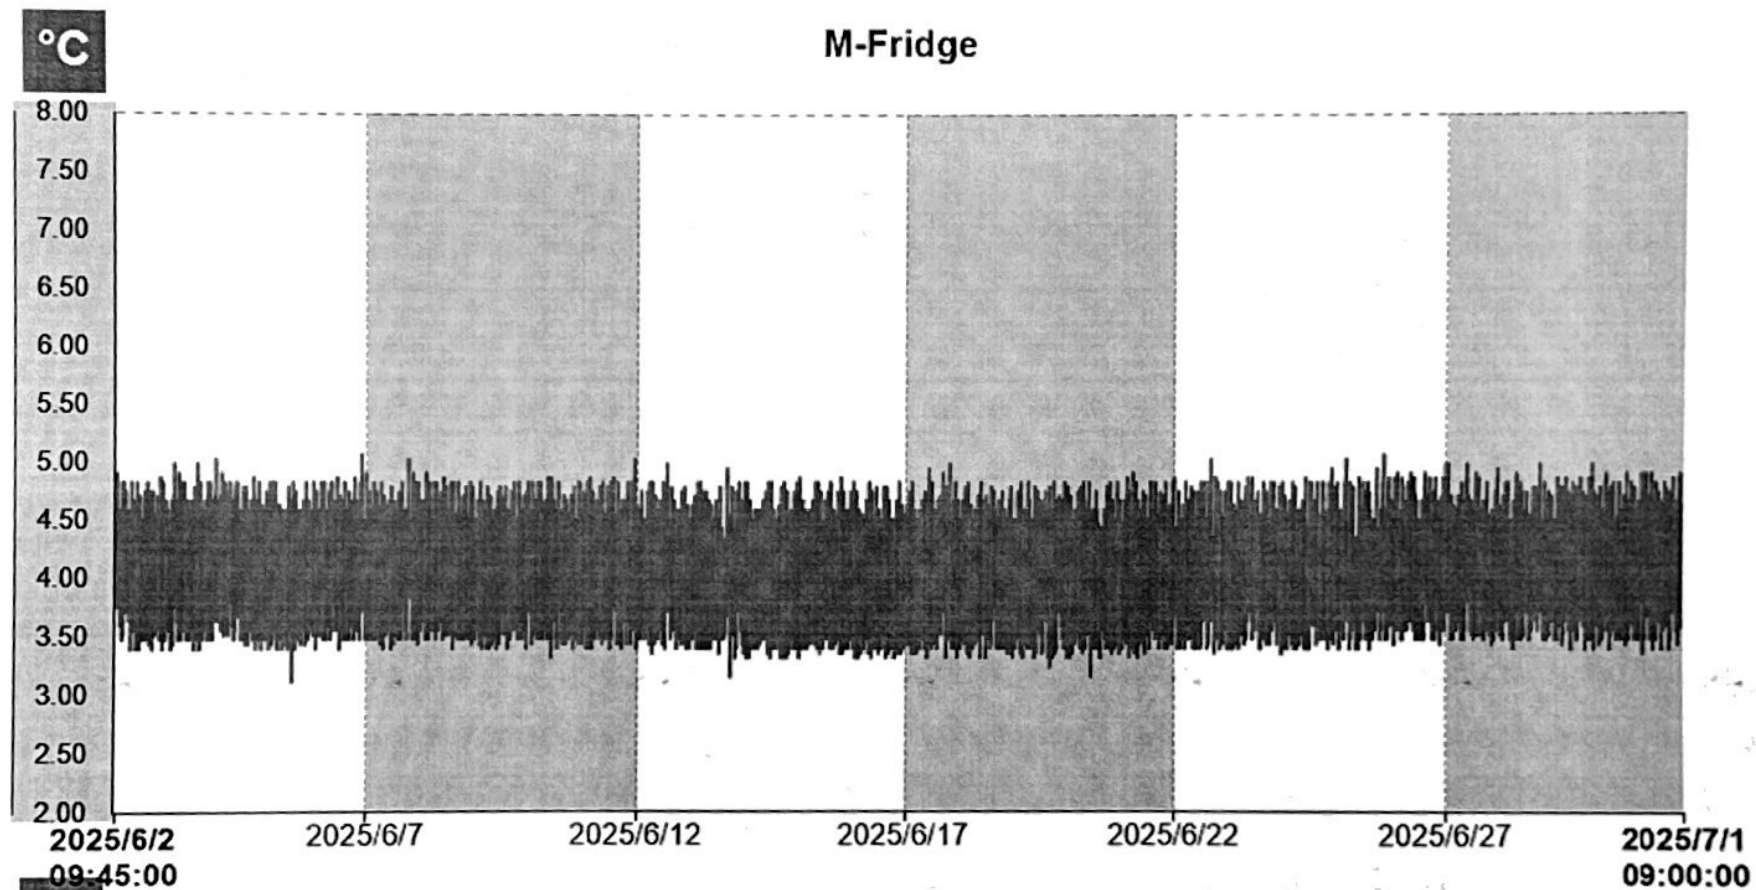

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07542]						
Ch-int1 M□□ [°C]	2782	3.1	5.1	4.09	0.49	4.11