

Chih-I Wy
2025-08-01



M-Fridge back up

2025/8/1 08:58:24

Device

Type of device
KH 50

Serial n°
OK 16.05.07540

Software version
1.06

Dataset parameters

Dataset name
M-Fridge back up

Type of dataset
Instant

Number of points
2977

Interval
15 minute(s)

Start date
2025/7/1 08:45:00

End date
2025/8/1 08:45:00

Comments

Channels

Channel
Ch-int1 M-Fridge [°C]

Measure
Temperature

Probe
Ambient thermo-hygro

Low threshold
2.0

High threshold
8.0


Minimum
3.0

Maximum
5.2

Average
4.12

Standard
0.59

MKT
4.14

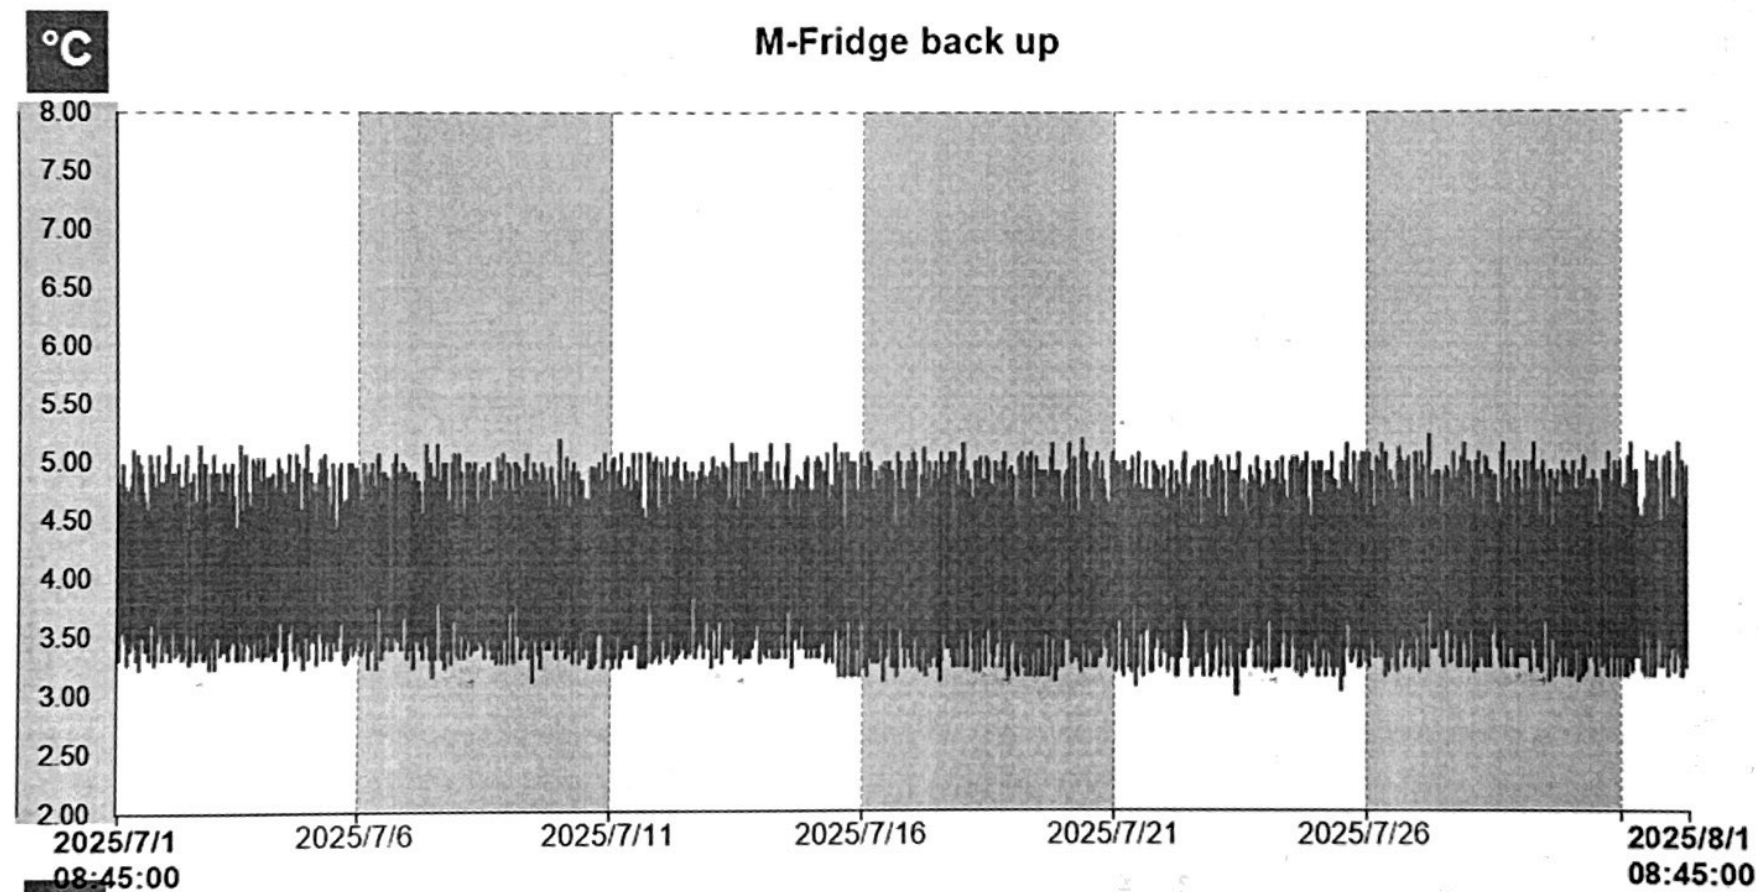



M-Fridge back up
2025/8/1 08:58:24

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07540] Ch-int1 M-Fridge [°C]	2977	3.0	5.2	4.12	0.59	4.14