



M-Fridge
2025/9/1 08:58:31

Device

Type of device	Serial n°	Software version
KH 50	OK 16.05.07542	1.06


Dataset parameters

Dataset name	Type of dataset
M-Fridge	Instant
Number of points	Interval
4320	15 minute(s)
Start date	End date
2025/7/18 09:00:00	2025/9/1 08:45:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 M□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
2.6	5.1	3.95
		Standard
		0.62
		MKT
		3.97

2025/9/1 08:58:31
M-Fridge

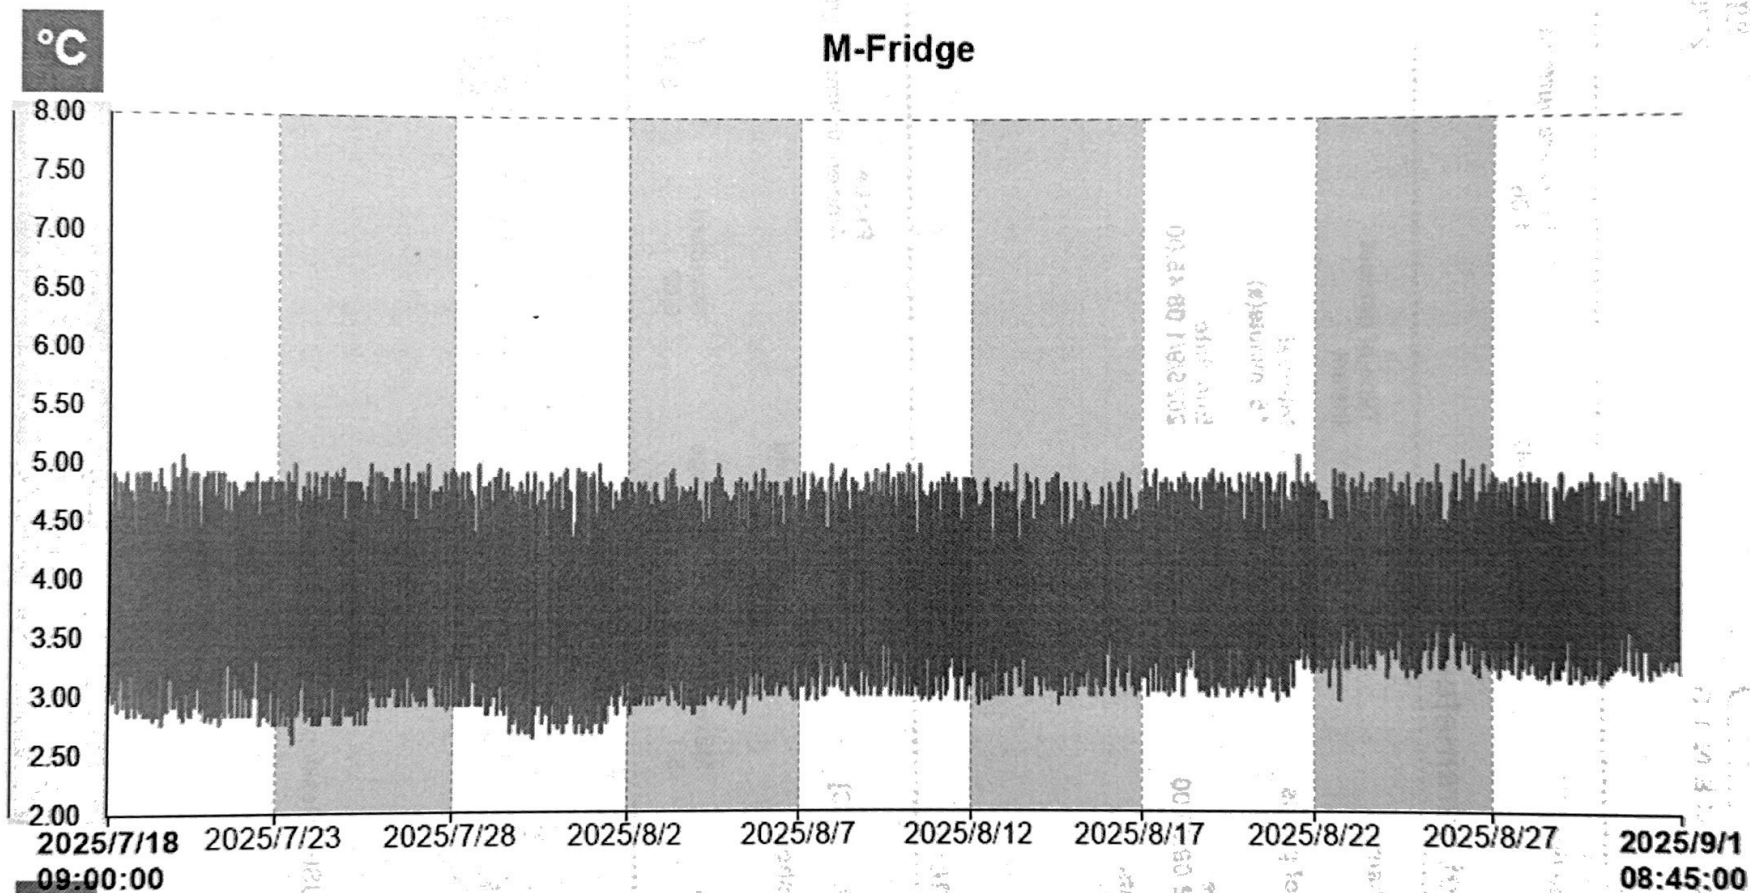

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07542] Ch-int1 M [°C]	4320	2.6	5.1	3.95	0.62	3.97