

Chih-I Wu
01 Oct 2025



M-Fridge back up

2025/10/1 09:50:38

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07540	1.06

Dataset parameters

Dataset name	Type of dataset
M-Fridge back up	Instant
Number of points	Interval
4072	15 minute(s)
Start date	End date
2025/8/20 00:00:00	2025/10/1 09:45:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 M-Fridge [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
2.8	5.1	4.21
		Standard
		0.56
		MKT
		4.22

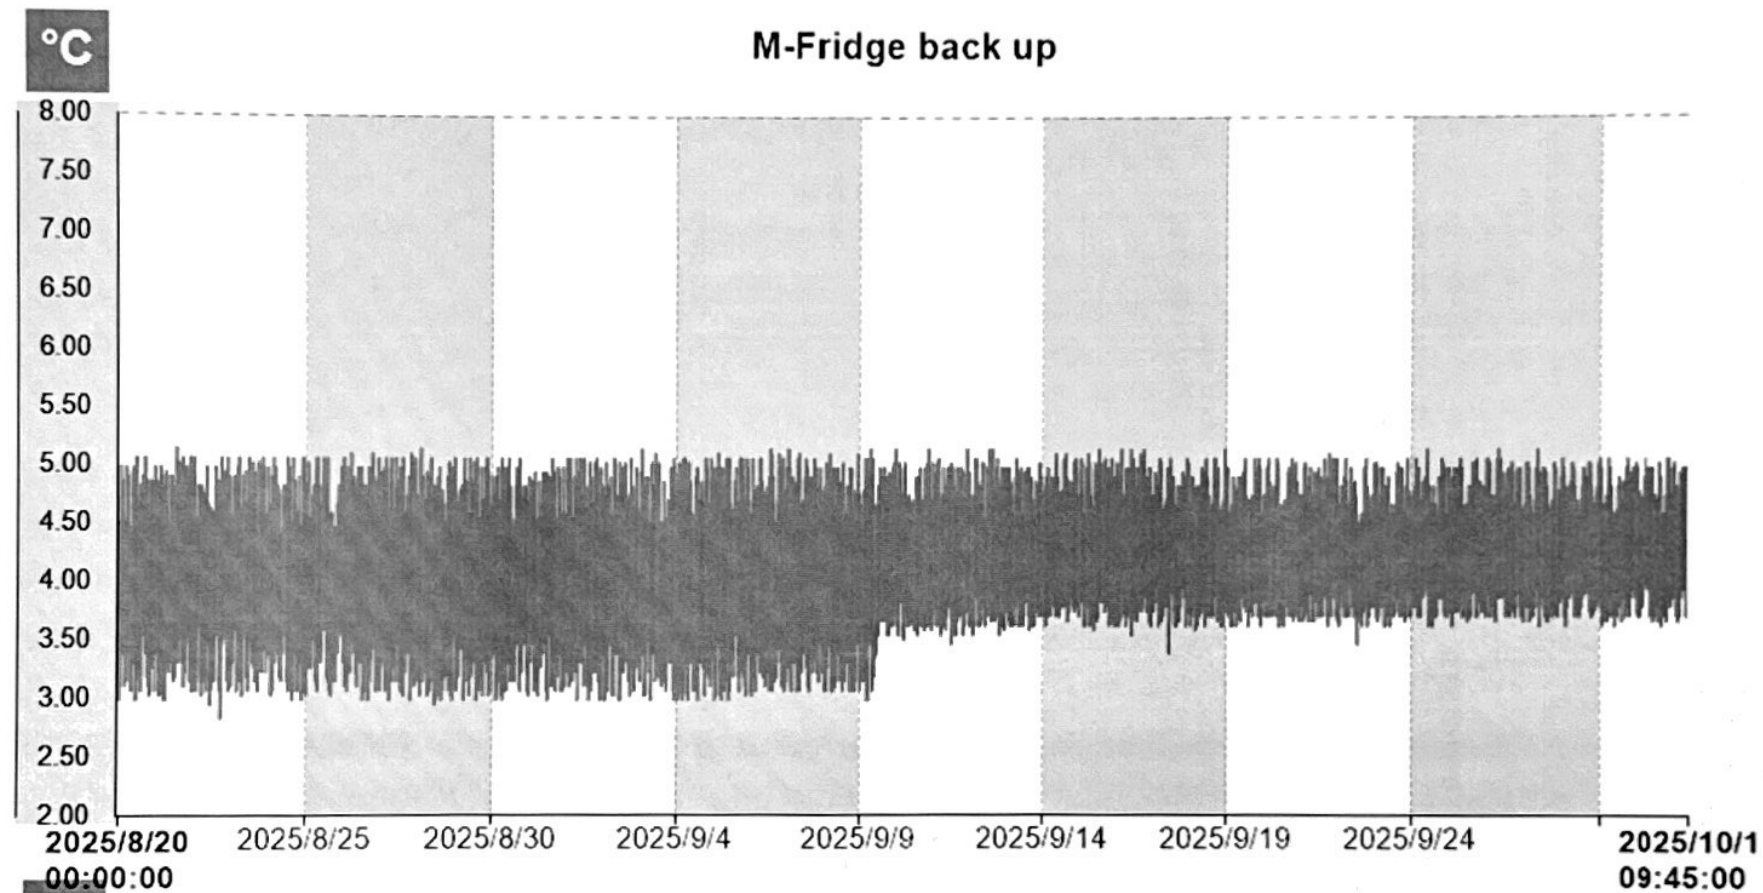



M-Fridge back up

2025/10/1 09:50:38

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07540] Ch-int1 M-Fridge [°C]	4072	2.8	5.1	4.21	0.56	4.22