

Chih-I Wu
03 Nov 2025



M-Fridge
2025/11/3 10:31:34

Device


Type of device	Serial n°	Software version
KH 50	OK 16.05.07542	1.06

Dataset parameters

Dataset name	Type of dataset
M-Fridge	Instant
Number of points	Interval
6052	15 minute(s)
Start date	End date
2025/9/1 09:30:00	2025/11/3 10:15:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 M□□ [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.1	5.4	4.17
		Standard
		0.48
		MKT
		4.18

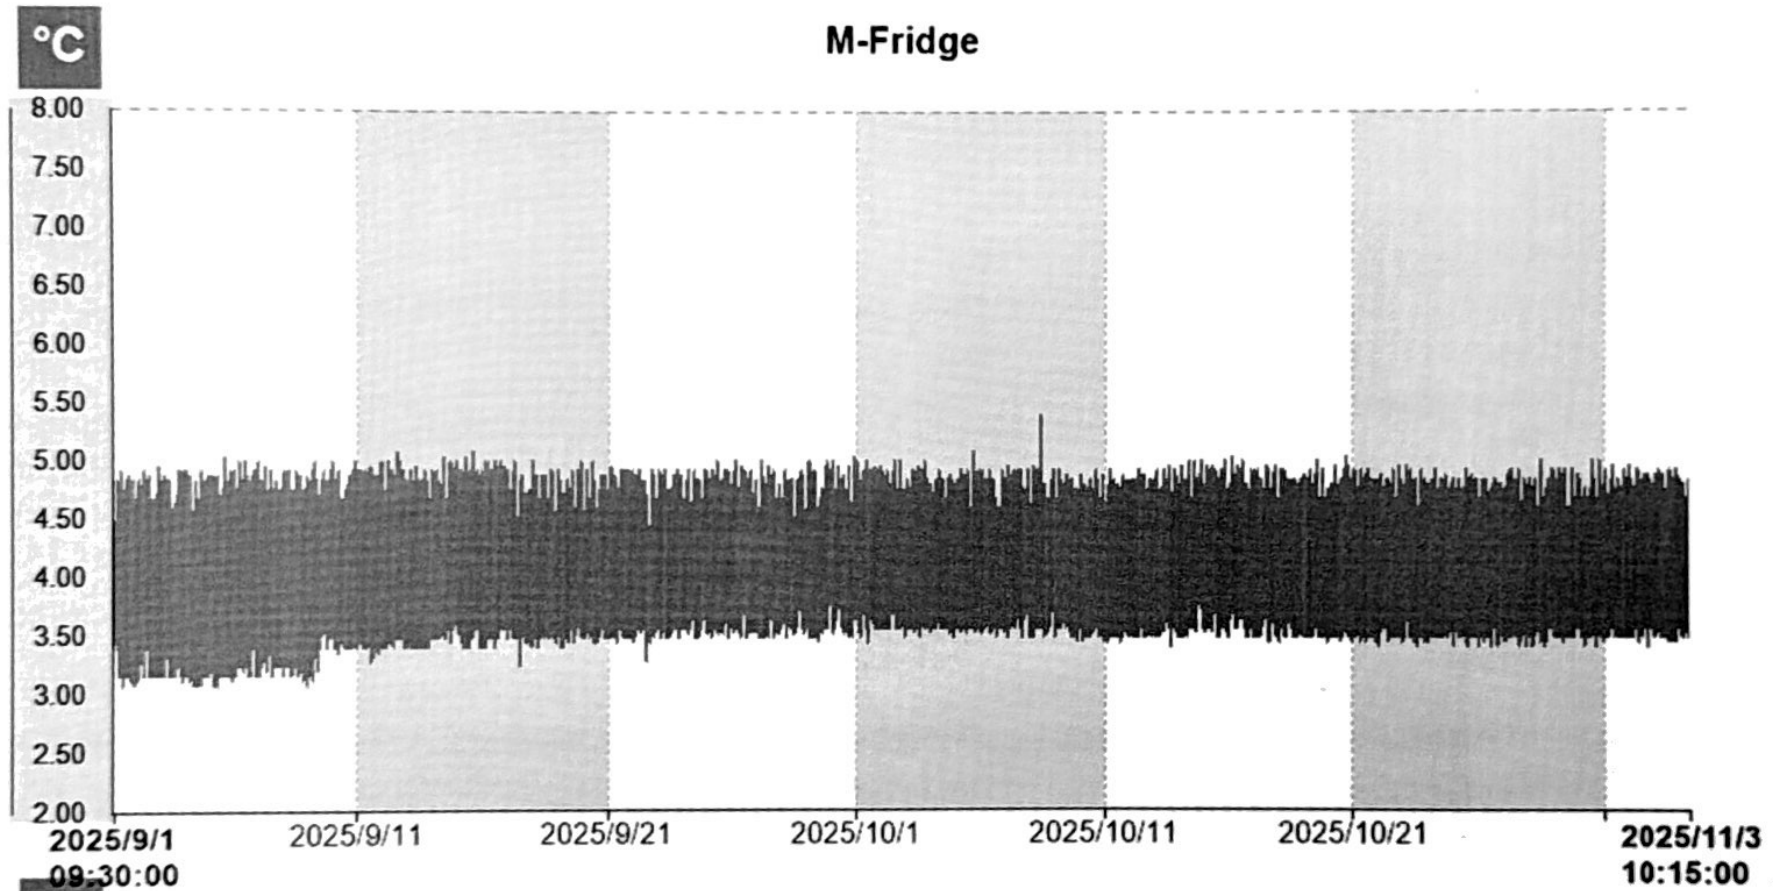



M-Fridge
2025/11/3 10:31:34

		Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07542]							
Ch-int1 M	[C]	6052	3.1	5.4	4.17	0.48	4.18