



M-Fridge
2026/1/2 11:18:01

Device

Type of device KH 50	Serial n° OK 16.05.07542	Software version 1.06
-------------------------	-----------------------------	--------------------------


Dataset parameters

Dataset name M-Fridge	Type of dataset Instant
Number of points 5762	Interval 15 minute(s)
Start date 2025/11/3 10:50:00	End date 2026/1/2 11:05:00
Comments	

Channels

Channel Ch-int1 M□□ [°C]	Measure Temperature	Probe Ambient thermo-hygro		
Low threshold 2.0	High threshold 8.0			
Minimum 3.2	Maximum 5.7	Average 4.15	Standard 0.51	MKT 4.16

Old 7-401's
down on 1/2

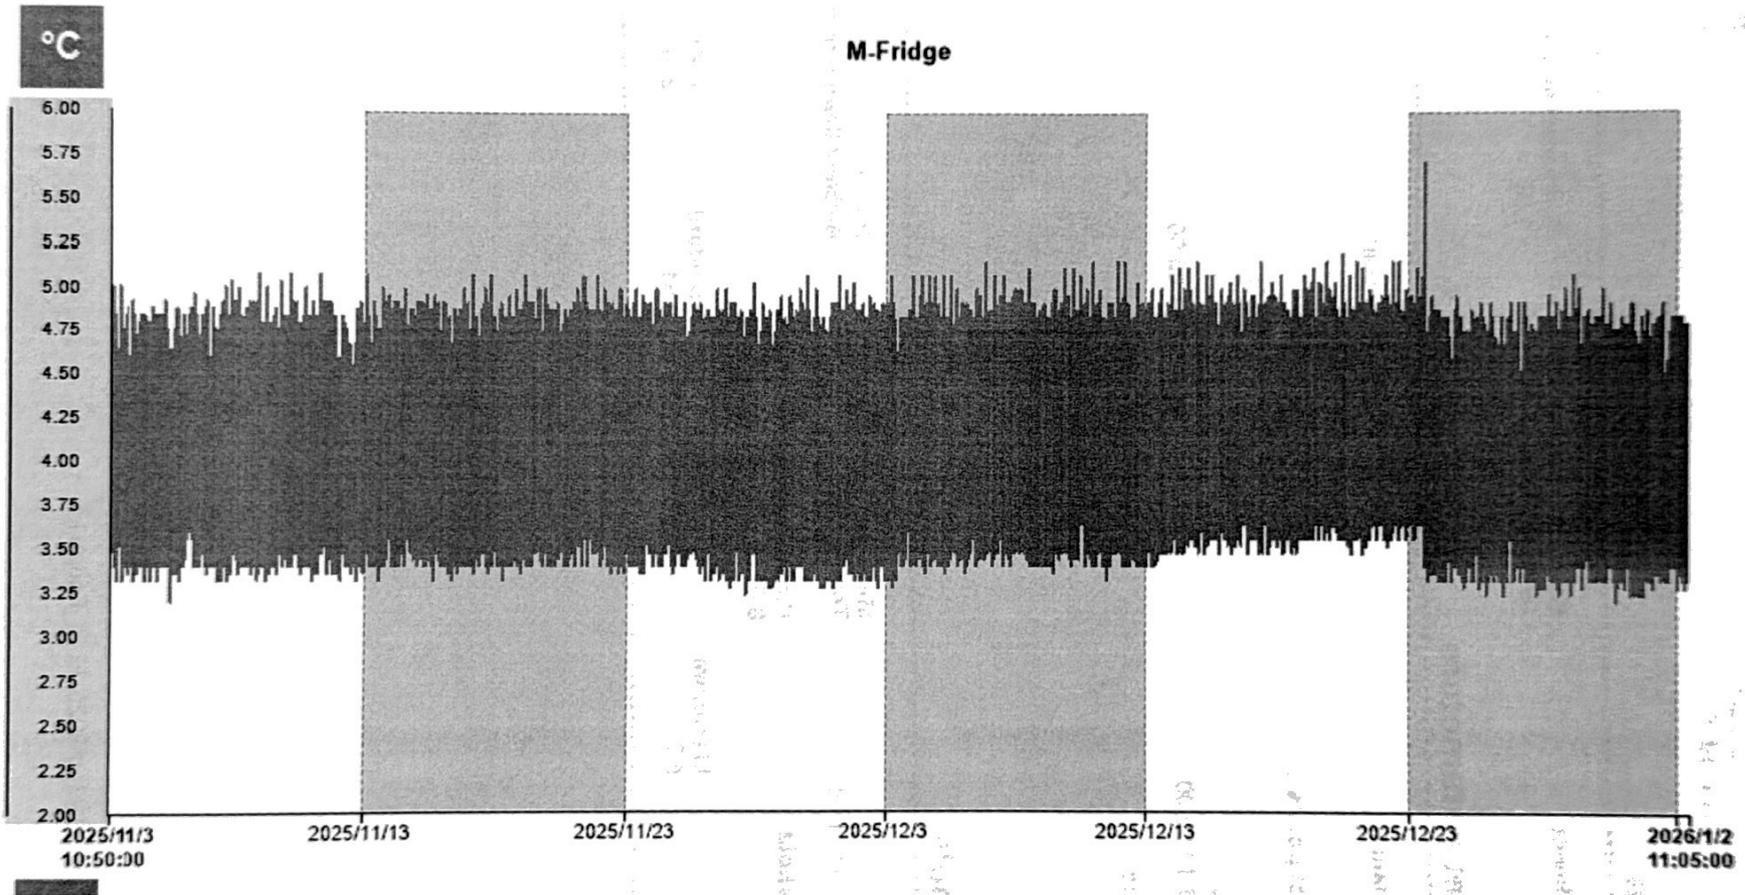



M-Fridge
2026/1/2 11:18:01

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.05.07542] Ch-int1 M□□ [°C]	5762	3.2	5.7	4.15	0.51	4.16