



INSTRUMENTS

M-Fridge

2026/3/2 09:49:35

Device


Type of device KH 50	Serial n° OK 16.05.07542	Software version 1.06
-------------------------	-----------------------------	--------------------------

Dataset parameters

Dataset name M-Fridge	Type of dataset Instant
Number of points 5657	Interval 15 minute(s)
Start date 2026/1/2 11:40:00	End date 2026/3/2 09:40:00
Comments	

Channels

Channel Ch-int1 M□□ [°C]	Measure Temperature	Probe Ambient thermo-hygro
Low threshold 2.0	High threshold 8.0	
Minimum 3.0	Maximum 5.8	Average 4.08
		Standard 0.50
		MKT 4.09

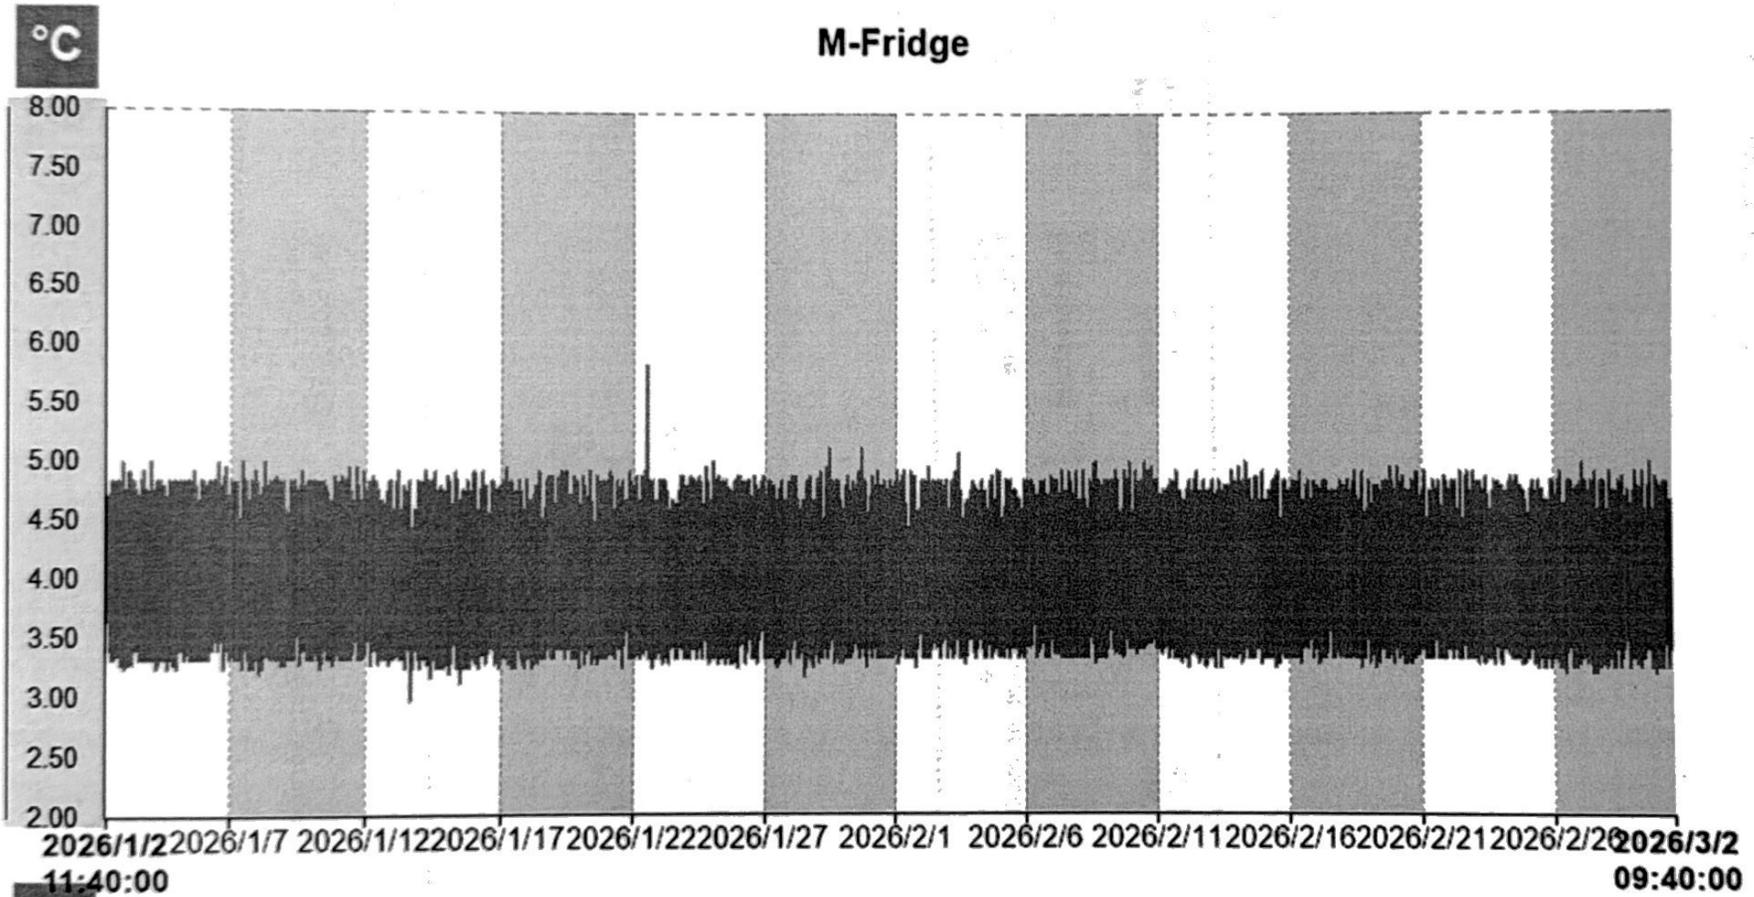



M-Fridge
2026/3/2 09:49:35

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH.50 [OK 16.05.07542] Ch-int1 M 11 [°C]	5657	3.0	5.8	4.08	0.50	4.09