

**M-Fridge**  
2024/4/1 09:10:41**Device**


|                |                |                  |
|----------------|----------------|------------------|
| Type of device | Serial n°      | Software version |
| KH 50          | OK 16.05.07542 | 1.06             |

**Dataset parameters**

|                   |                   |
|-------------------|-------------------|
| Dataset name      | Type of dataset   |
| M-Fridge          | Instant           |
| Number of points  | Interval          |
| 2971              | 15 minute(s)      |
| Start date        | End date          |
| 2024/3/1 10:30:00 | 2024/4/1 09:00:00 |
| Comments          |                   |

**Channels**

|                  |                |                      |          |      |
|------------------|----------------|----------------------|----------|------|
| Channel          | Measure        | Probe                |          |      |
| Ch-int1 M□□ [°C] | Temperature    | Ambient thermo-hygro |          |      |
| Low threshold    | High threshold |                      |          |      |
| 2.0              | 8.0            |                      |          |      |
| Minimum          | Maximum        | Average              | Standard | MKT  |
| 4.0              | 5.6            | 4.55                 | 0.31     | 4.55 |

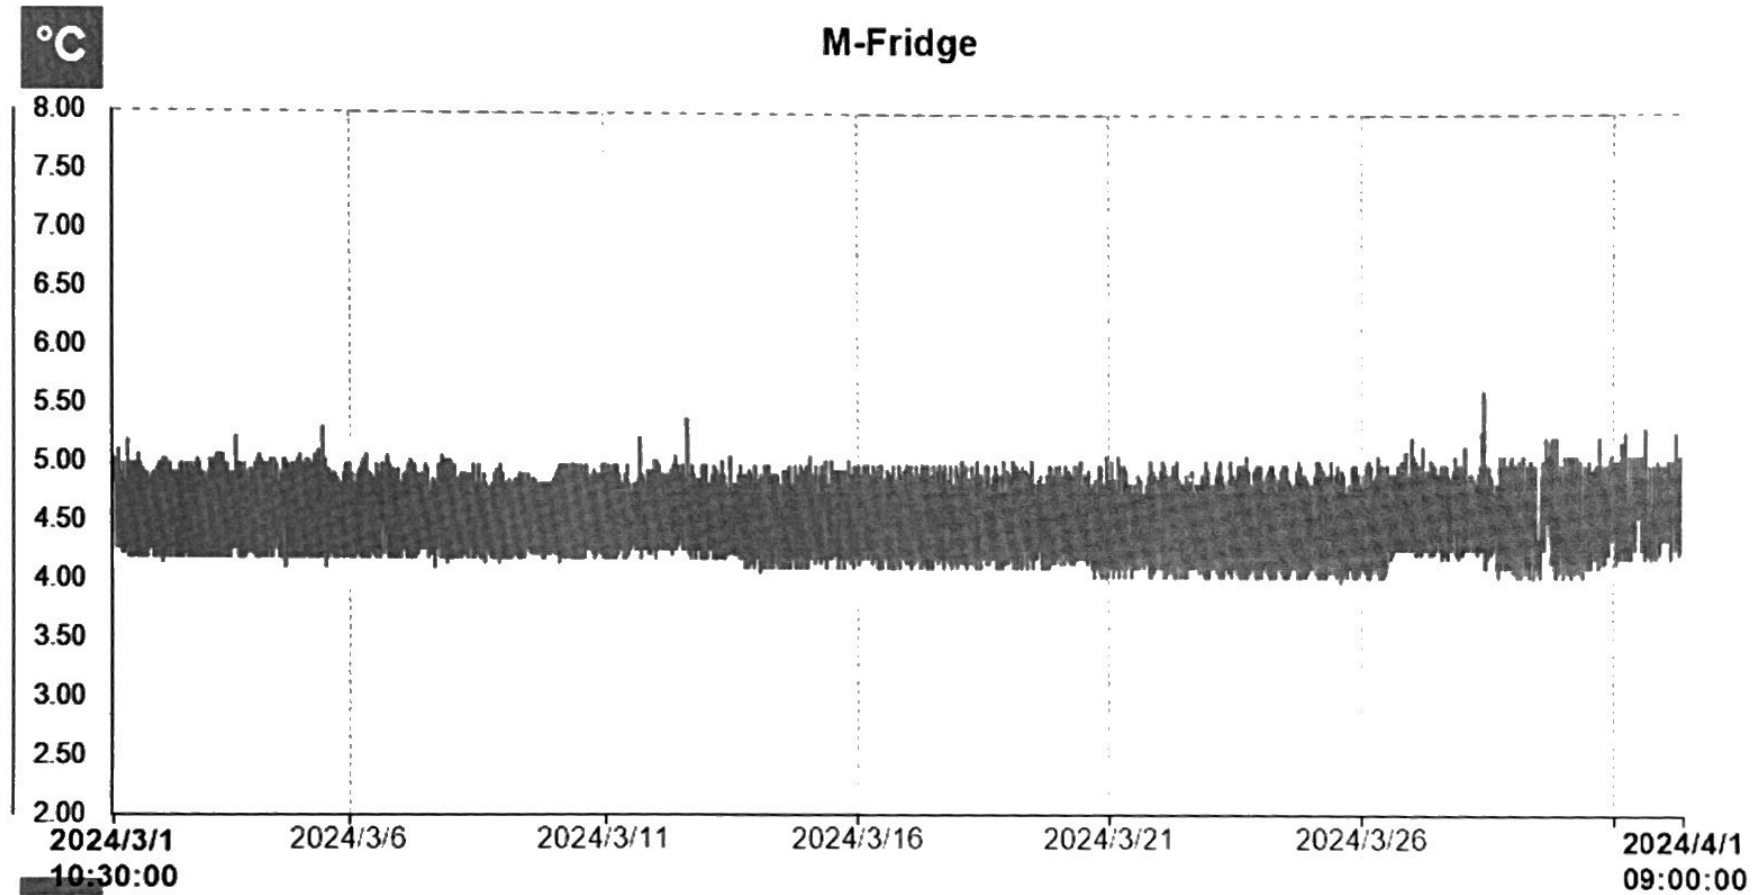



M-Fridge  
2024/4/1 09:10 41

|                                               |  | Number of<br>points | Minimum | Maximum | Average | Standard<br>deviation | MKT  |
|-----------------------------------------------|--|---------------------|---------|---------|---------|-----------------------|------|
| KH 50 [OK 16.05.07542]<br>Ch-int1 M      [°C] |  | 2971                | 4.0     | 5.6     | 4.55    | 0.31                  | 4.55 |