



M-Fridge back up

2026/2/2 08:37:24

Device


Type of device KH 50	Serial n° 0K 16.05.07540	Software version 1.06
-------------------------	-----------------------------	--------------------------

Dataset parameters

Dataset name M-Fridge back up	Type of dataset Instant
Number of points 6040	Interval 15 minute(s)
Start date 2025/12/1 10:40:00	End date 2026/2/2 08:25:00
Comments	

Channels

Channel Ch-int1 M-Fridge [°C]	Measure Temperature	Probe Ambient thermo-hygro		
Low threshold 2.0	High threshold 8.0			
Minimum 2.9	Maximum 5.7	Average 4.09	Standard 0.57	MKT 4.11

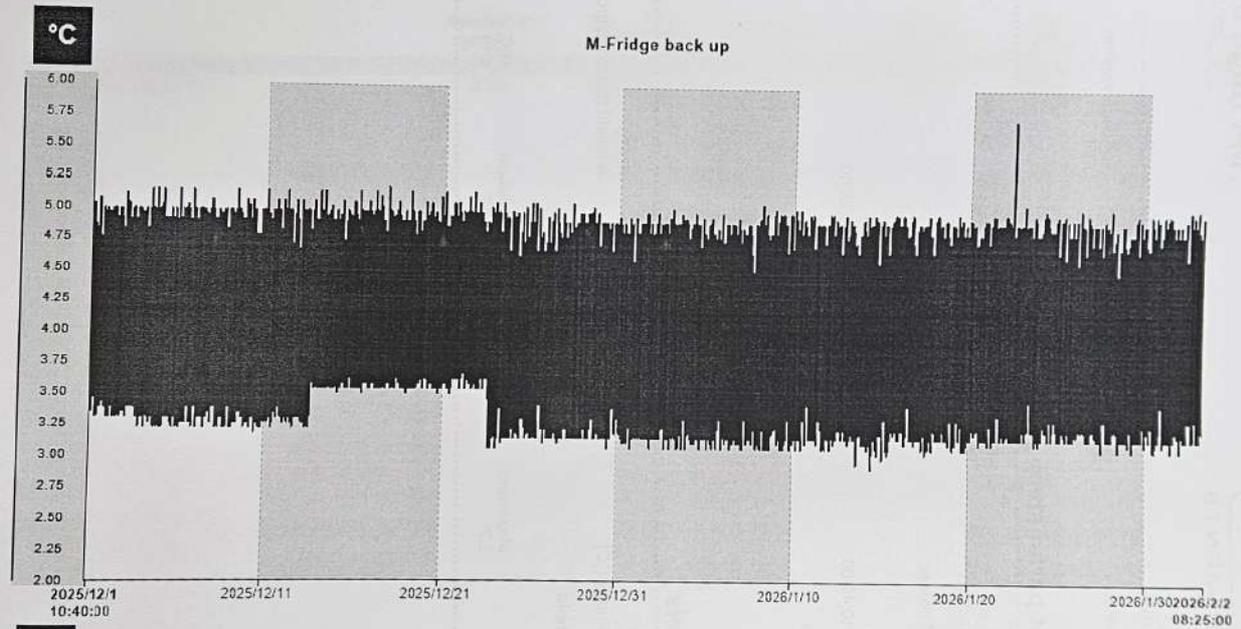



M-Fridge back up

2026/2/2 08:37:24

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH.50 [OK 16.05.07540] Ch-int1 M-Fridge [°C]	6040	2.9	5.7	4.09	0.57	4.11