



Chih-I Wu
01 May 2024

P-Fridge
2024/5/1 09:28:49

Device


Type of device	Serial n°	Software version
KH 50	OK 16.12.12000	1.06

Dataset parameters

Dataset name	Type of dataset
P-Fridge	Instant
Number of points	Interval
2881	15 minute(s)
Start date	End date
2024/4/1 09:25:00	2024/5/1 09:25:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.4	5.2	4.38
		Standard
		0.34
		MKT
		4.39

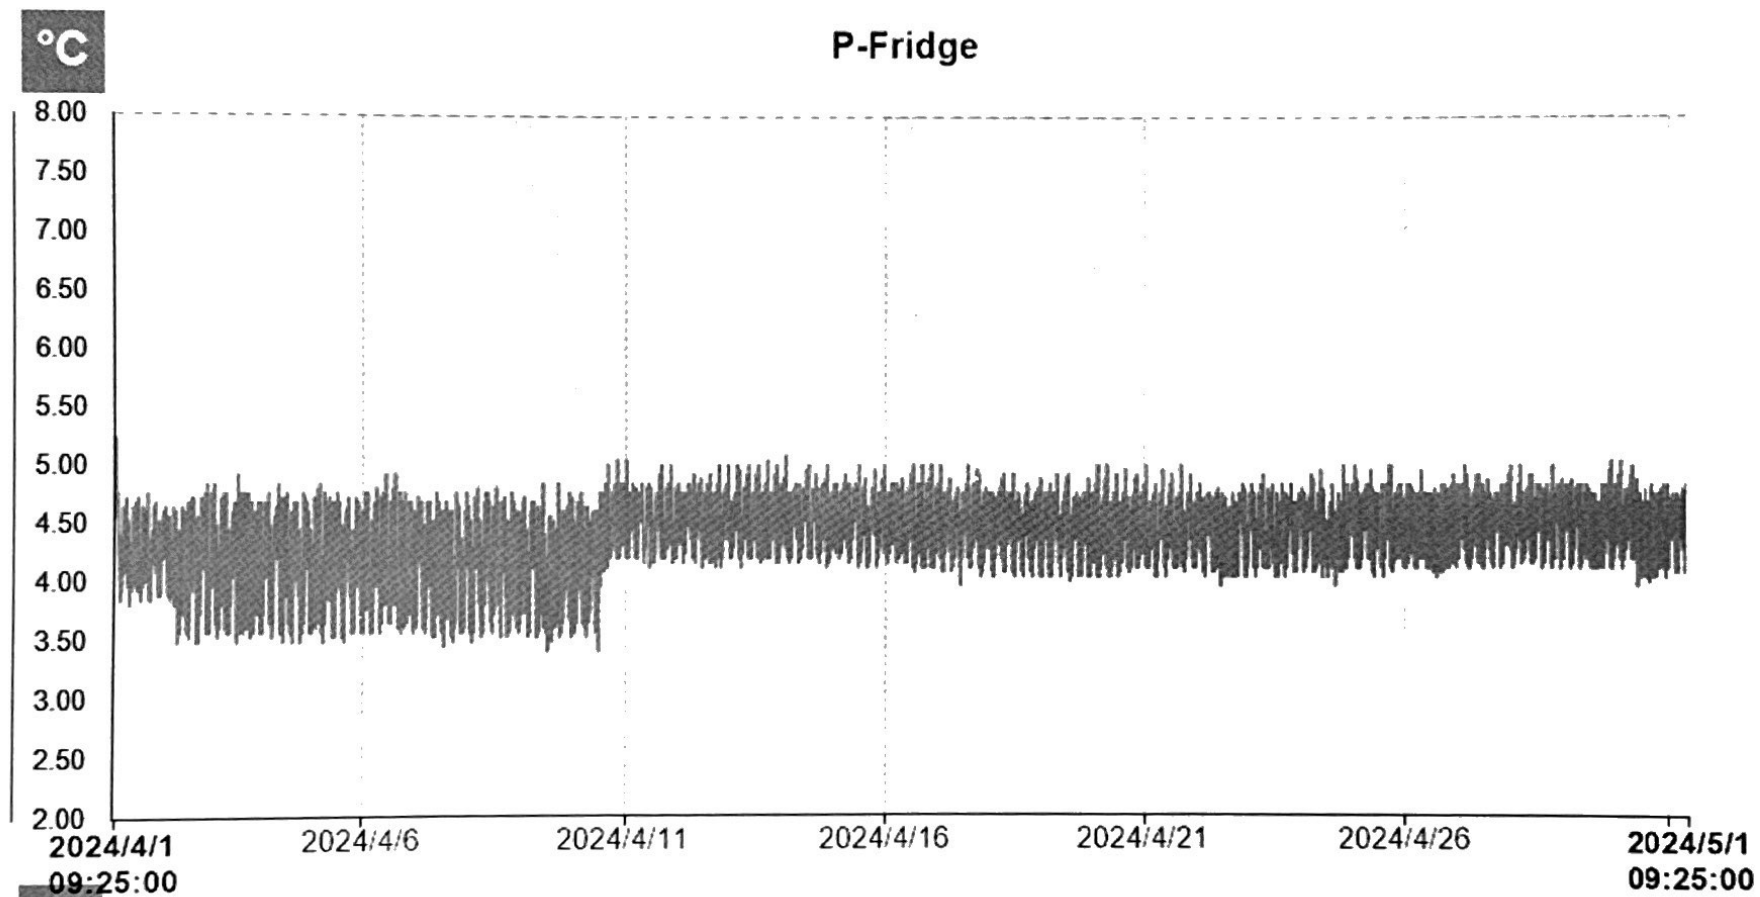

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.12.12000]						
Ch-int1 [°C]	2881	3.4	5.2	4.38	0.34	4.39