



P-Fridge
2024/11/1 09:39:58

Device


Type of device	Serial n°	Software version
KH 50	OK 16.12.12000	1.06

Dataset parameters

Dataset name	Type of dataset
P-Fridge	Instant
Number of points	Interval
2955	15 minute(s)
Start date	End date
2024/10/1 15:05:00	2024/11/1 09:35:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
3.5	5.3	4.37	0.40	4.37

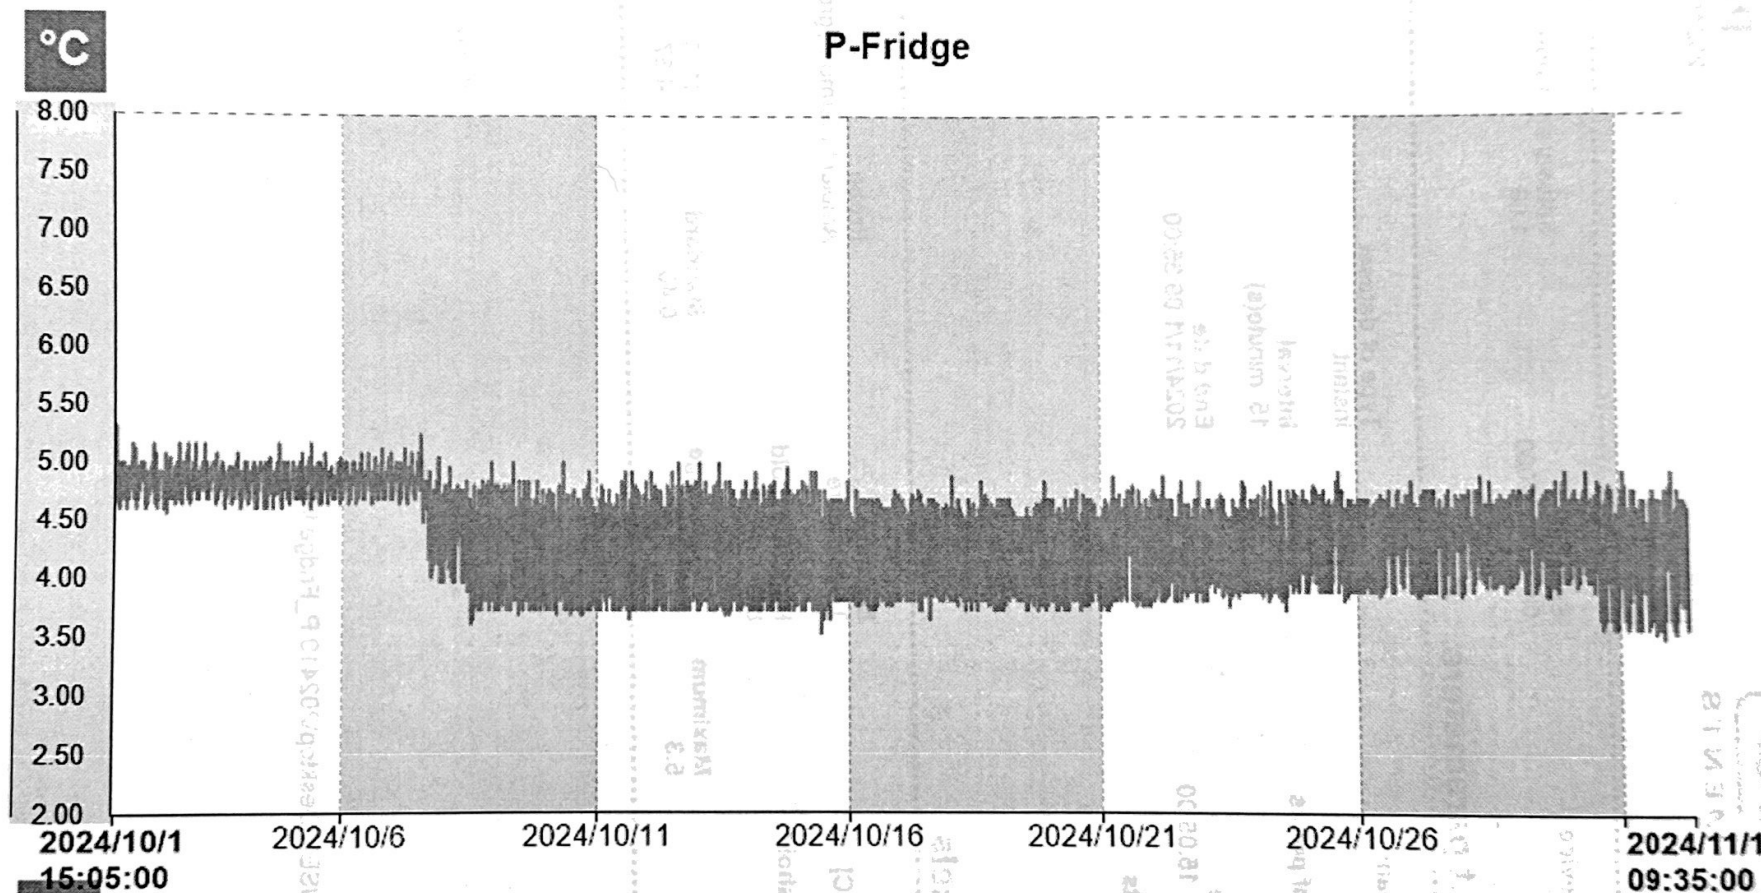



P-Fridge
2024/11/1 09:39:58

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [0K 16.12.12000]						
Ch-int1 [°C]	2955	3.5	5.3	4.37	0.40	4.37