



P-Fridge
2024/12/2 10.03.20

Device


Type of device	Serial n°	Software version
KH 50	OK 16.12.12000	1.06

Dataset parameters

Dataset name	Type of dataset
P-Fridge	Instant
Number of points	Interval
2976	15 minute(s)
Start date	End date
2024/11/1 10:10:00	2024/12/2 09:55:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
2.9	5.4	4.09
		Standard
		0.52
		MKT
		4.11

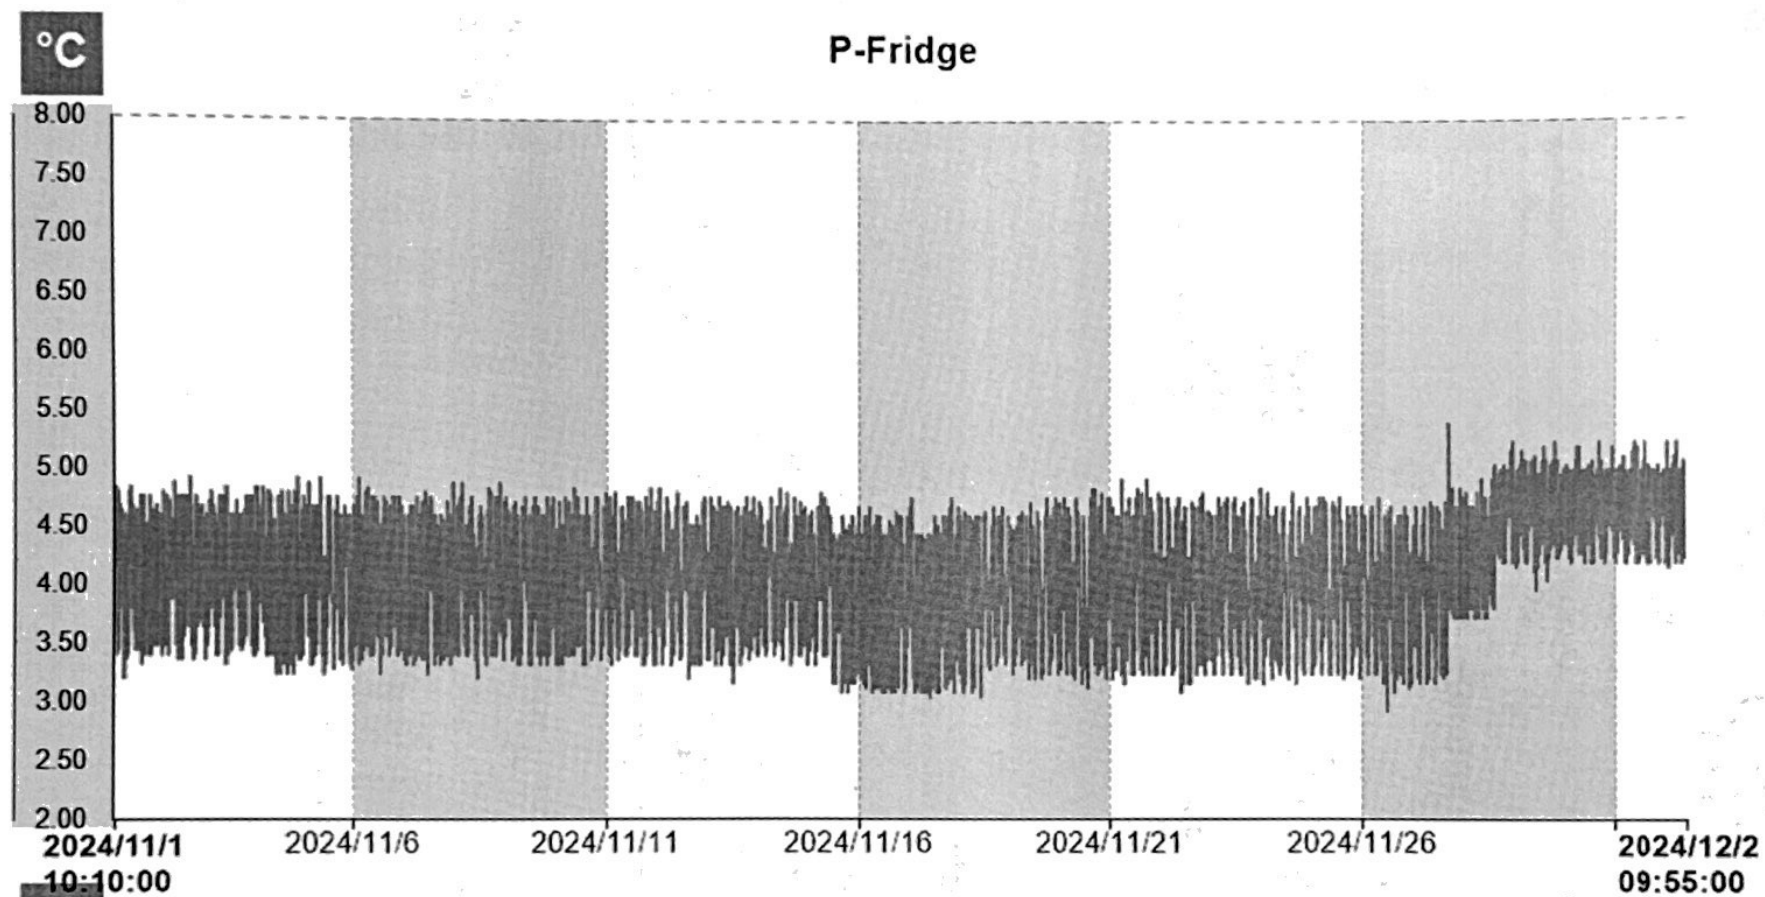



P-Fridge
2024/12/2 10:03:20

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.12.12000]						
Ch-int1 [°C]	2976	2.9	5.4	4.09	0.52	4.11