



P-Fridge
2025/1/2 10:02:17

Device


Type of device	Serial n°	Software version
KH 50	OK 16.12.12000	1.06

Dataset parameters

Dataset name	Type of dataset
P-Fridge	Instant
Number of points	Interval
2975	15 minute(s)
Start date	End date
2024/12/2 10:25:00	2025/1/2 09:55:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.4	6.0	4.59
		Standard
		0.38
		MKT
		4.60

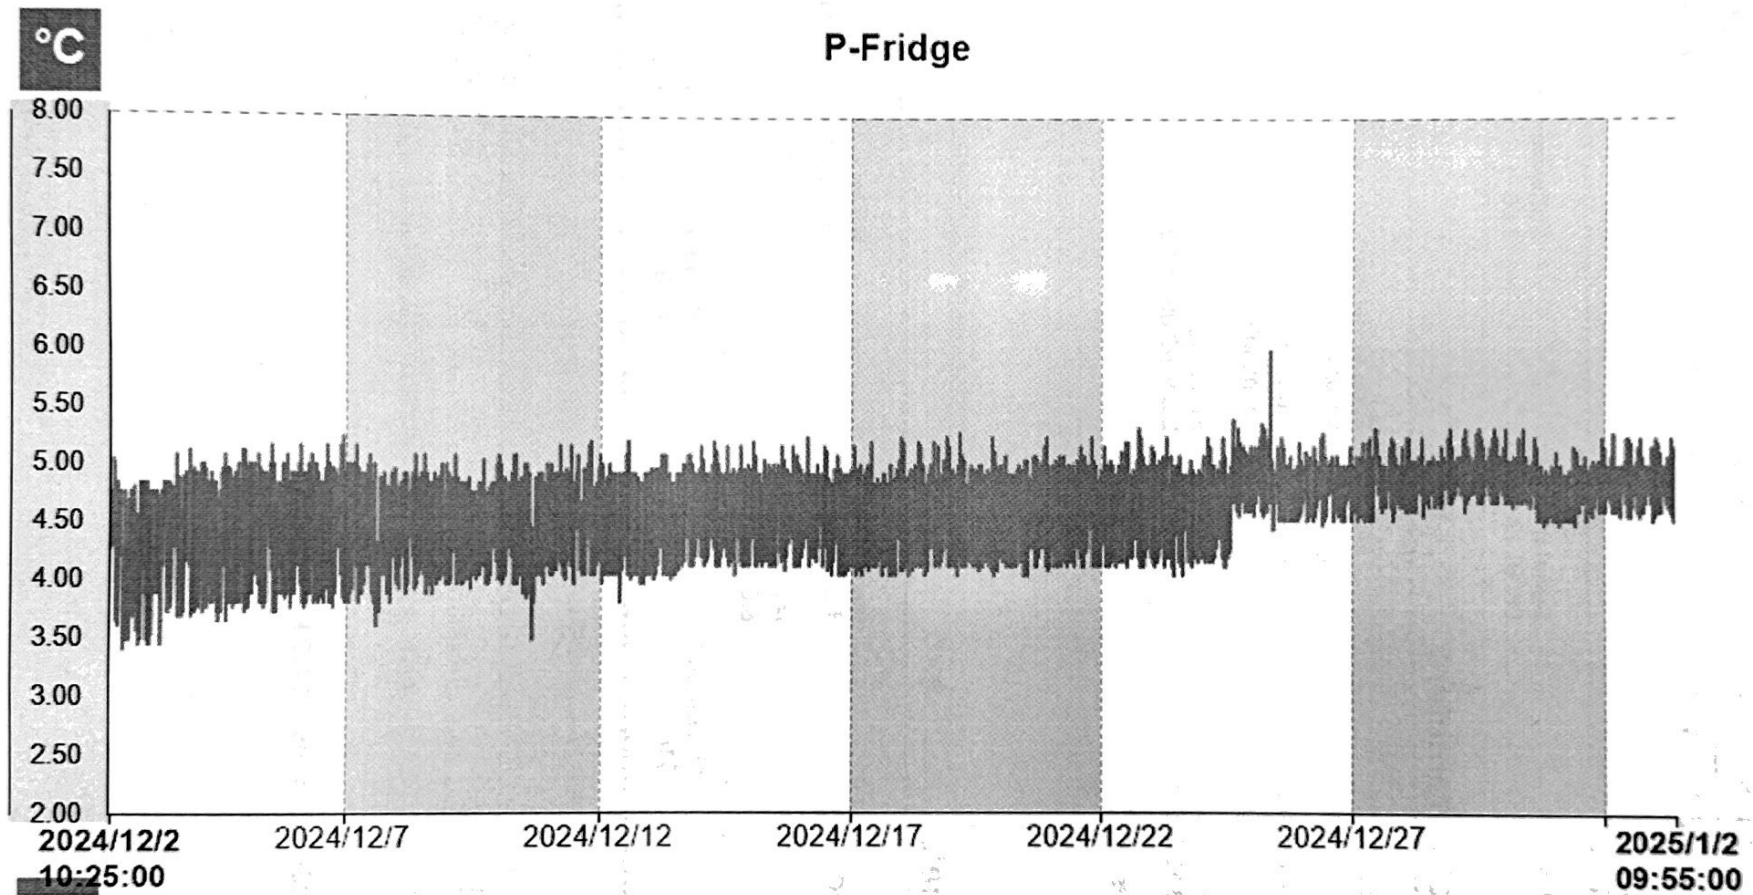



P-Fridge
2025/1/2 10:02:17

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.12.12000]						
Ch-int1 [°C]	2975	3.4	6.0	4.59	0.38	4.60