



P-Fridge
2025/2/3 10:26:23

Device

Type of device	Serial n°	Software version
KH 50	OK 16.12.12000	1.06


Dataset parameters

Dataset name	Type of dataset
P-Fridge	Instant
Number of points	Interval
3072	15 minute(s)
Start date	End date
2025/1/2 10:30:00	2025/2/3 10:15:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
4.1	6.1	4.81	0.27	4.81

02 EEP 5032
CMP-T 103

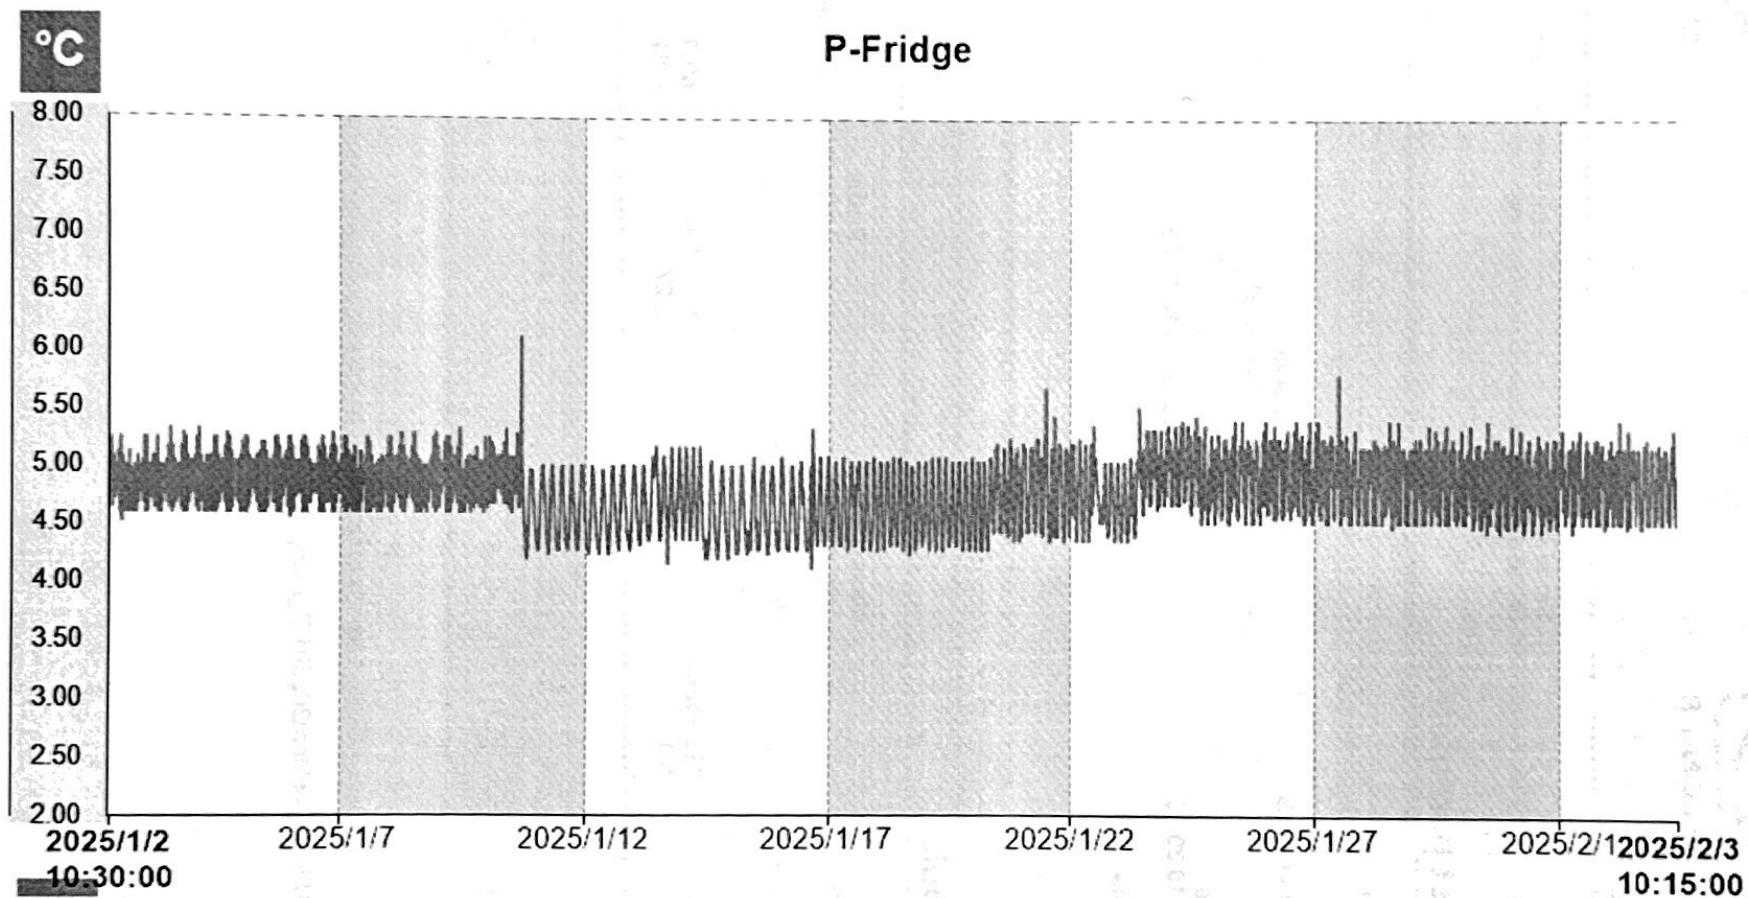



P-Fridge
2025/2/3 10:26:23

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.12.12000] Ch-int1 [°C]	3072	4.1	6.1	4.81	0.27	4.81