



P-Fridge
2025/3/3 09:03:15

Device

Type of device	Serial n°	Software version
KH 50	OK 16.12.12000	1.06


Dataset parameters

Dataset name	Type of dataset
P-Fridge	Instant
Number of points	Interval
2681	15 minute(s)
Start date	End date
2025/2/3 11:00:00	2025/3/3 09:00:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
3.8	6.3	4.53	0.37	4.54

31404-032
CWP-T 1AW

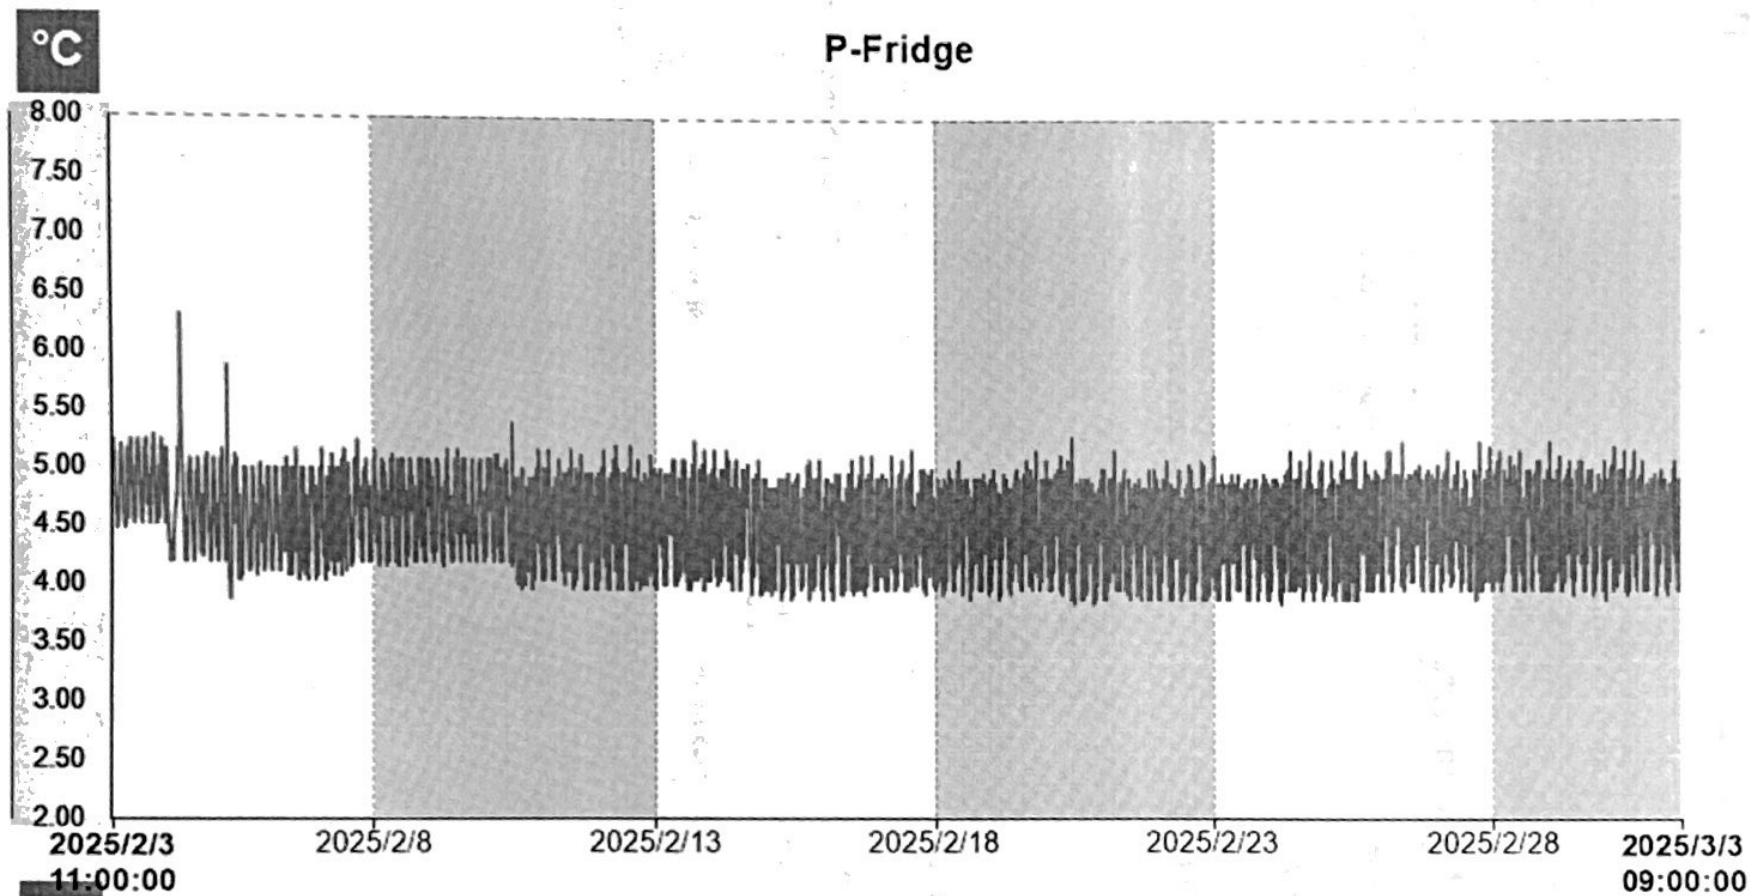

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.12.12000]						
Ch-int1 [°C]	2681	3.8	6.3	4.53	0.37	4.54