

Chih-I Wu
02 Apr 2025



P-Fridge
2025/4/2 09:36:10

Device


Type of device	Serial n°	Software version
KH 50	OK 16.12.12000	1.06

Dataset parameters

Dataset name	Type of dataset
P-Fridge	Instant
Number of points	Interval
2881	15 minute(s)
Start date	End date
2025/3/3 09:25:00	2025/4/2 09:25:00
Comments	

Channels

Channel	Measure	Probe
Ch-int1 [°C]	Temperature	Ambient thermo-hygro
Low threshold	High threshold	
2.0	8.0	
Minimum	Maximum	Average
3.5	5.2	4.33
		Standard
		0.34
		MKT
		4.34

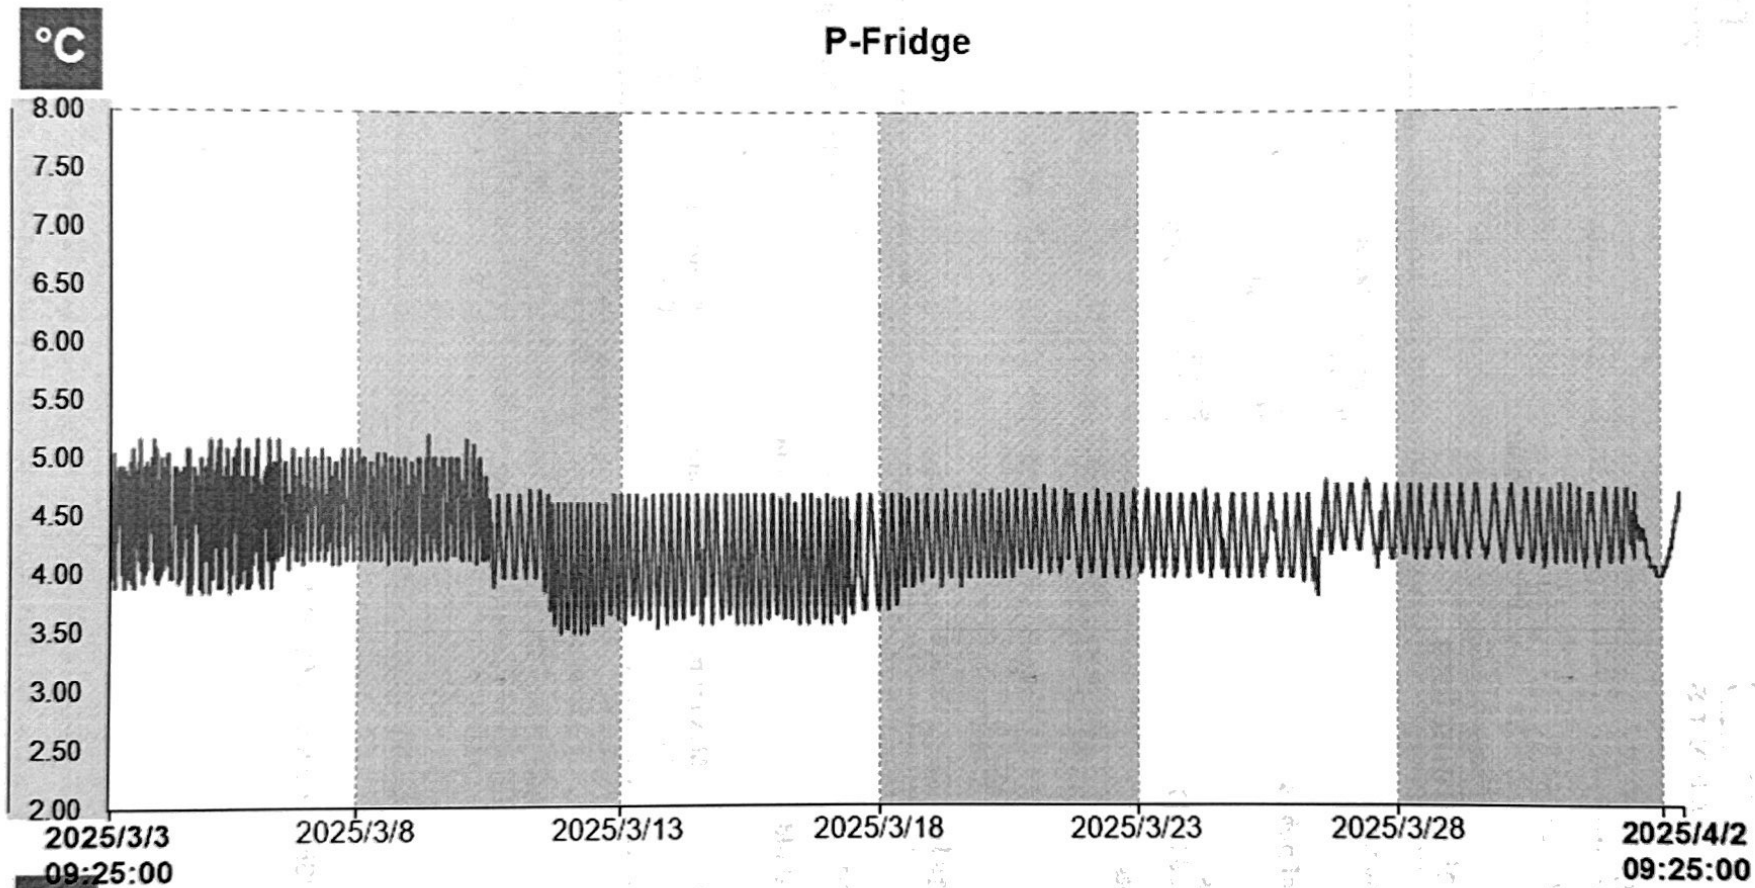

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.12.12000] Ch-int1 [°C]	2881	3.5	5.2	4.33	0.34	4.34