

Cuih - I Wu
01 Aug 2025



P Fridge backup

2025/8/1 08:56:36

Device


Type of device	Serial n°	Software version
KH 50	OK 17.12.19808	1.06

Dataset parameters

Dataset name	Type of dataset
P Fridge backup	Instant
Number of points	Interval
2978	15 minute(s)
Start date	End date
2025/7/1 08:40:00	2025/8/1 08:55:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
2.8	5.4	4.35	0.49	4.36

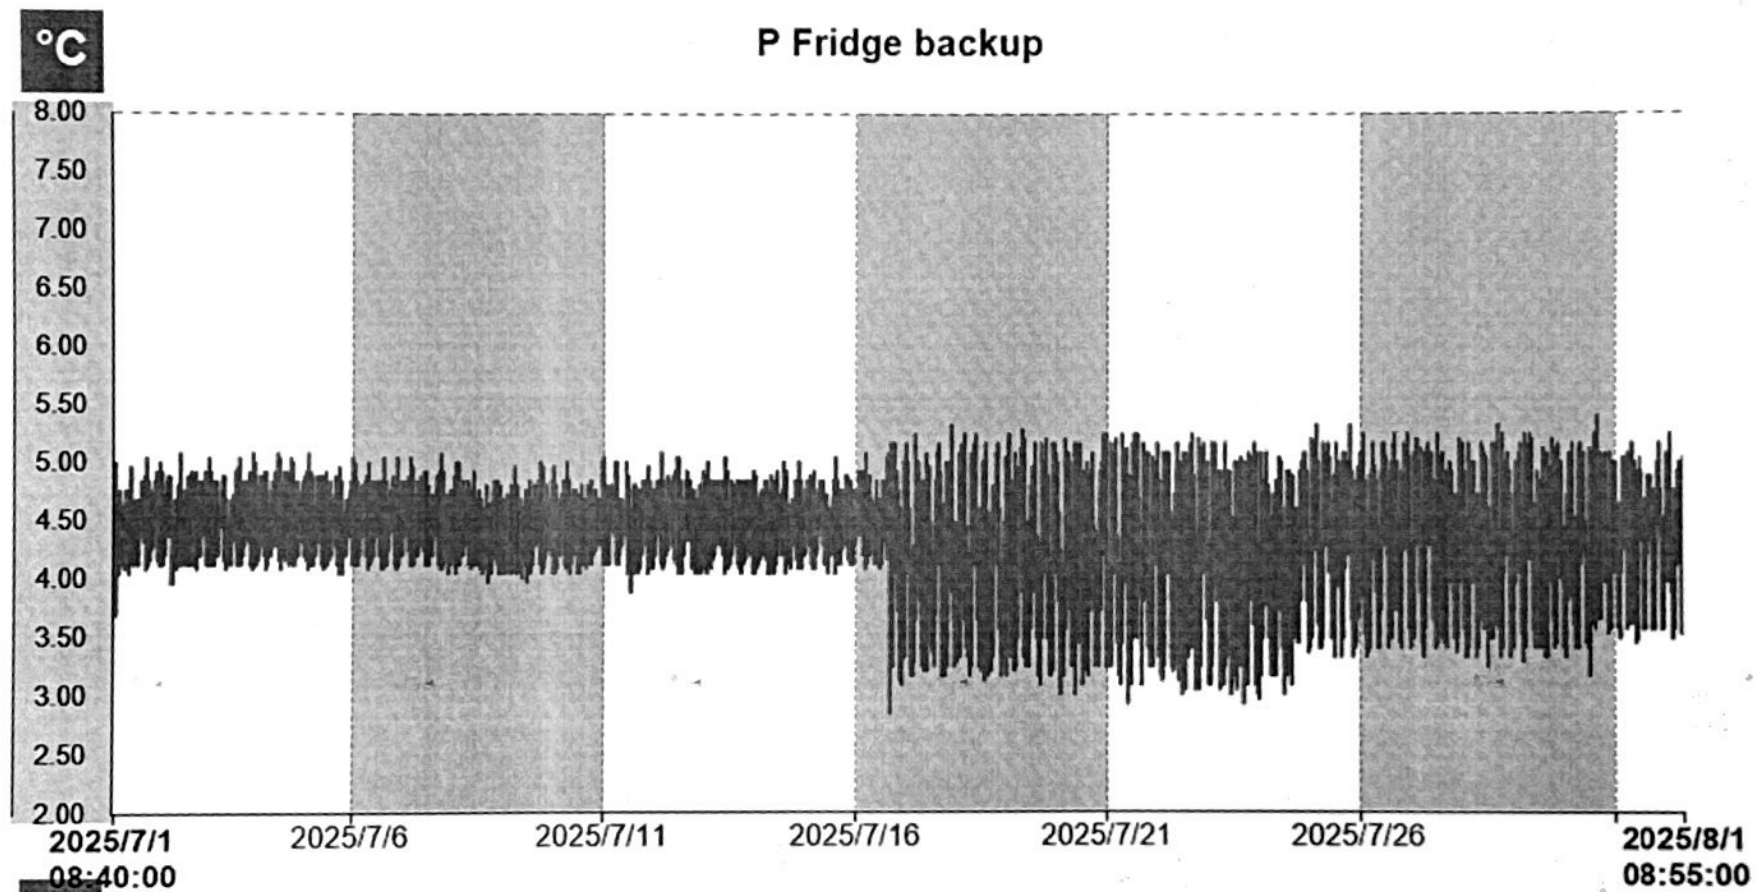



P Fridge backup

2025/8/1 08:56:36

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 17.12.19808]						
Ch-int1 [°C]	2978	2.8	5.4	4.35	0.49	4.36