

Chih-I Wu
03 Nov 2025



P-Fridge
2025/11/3 10:29:12

Device


Type of device	Serial n°	Software version
KH 50	OK 16.12.12000	1.06

Dataset parameters

Dataset name	Type of dataset
P-Fridge	Instant
Number of points	Interval
6052	15 minute(s)
Start date	End date
2025/9/1 09:40:00	2025/11/3 10:25:00
Comments	

Channels

Channel	Measure	Probe		
Ch-int1 [°C]	Temperature	Ambient thermo-hygro		
Low threshold	High threshold			
2.0	8.0			
Minimum	Maximum	Average	Standard	MKT
3.4	5.7	4.21	0.36	4.22

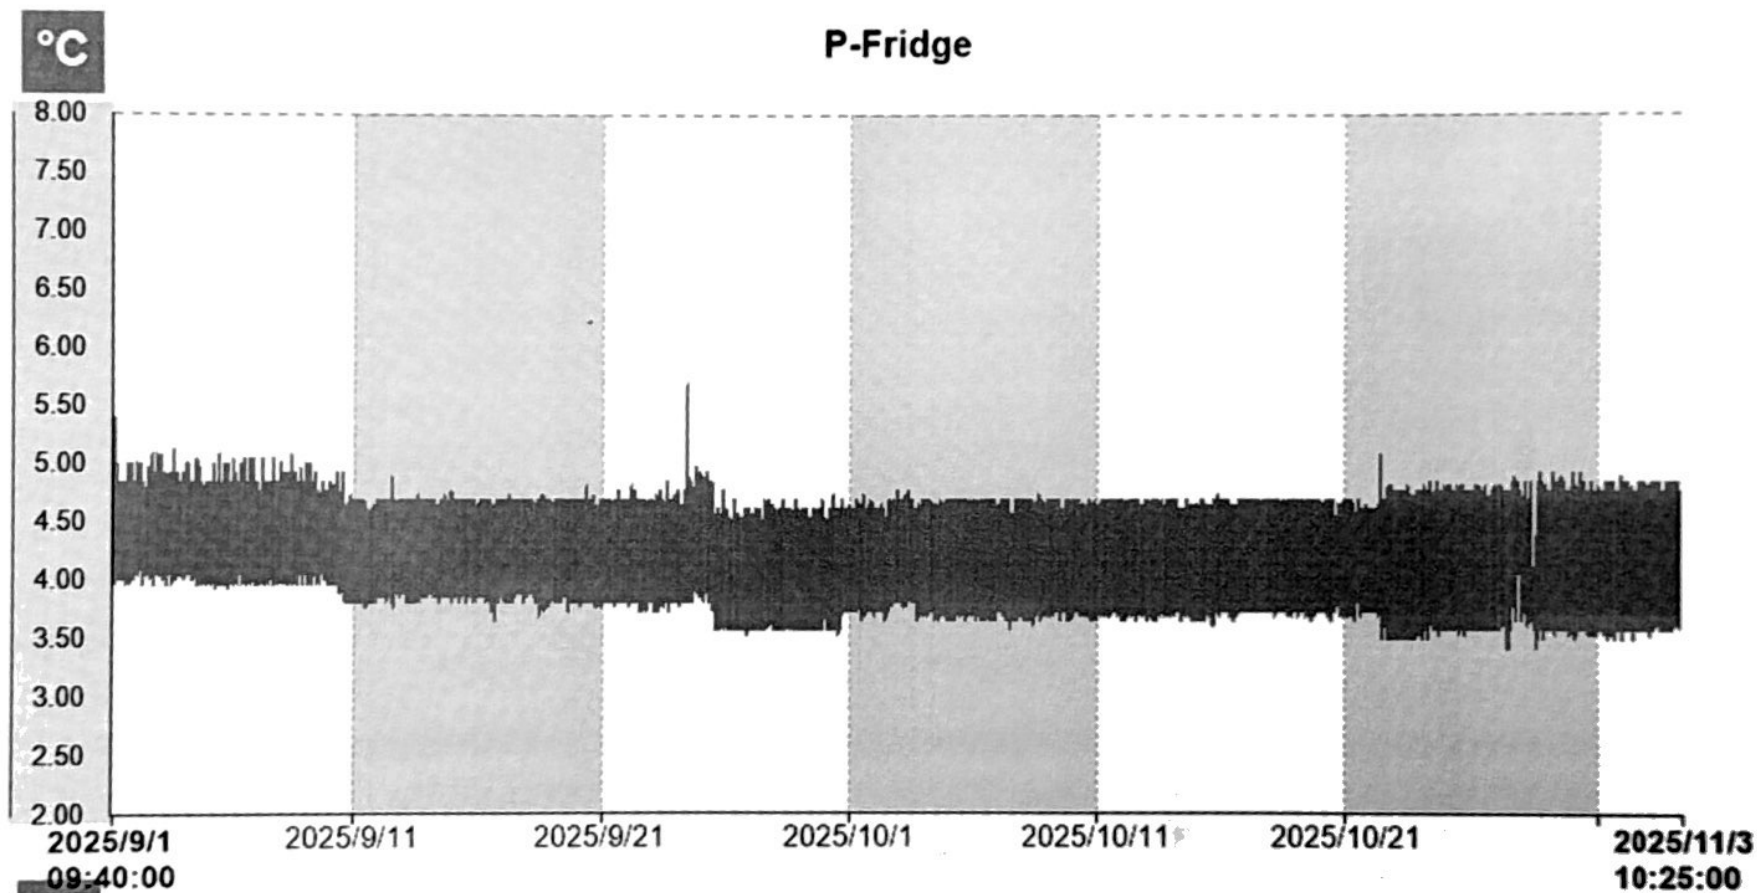

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.12.12000]						
Ch-int1 [°C]	6052	3.4	5.7	4.21	0.36	4.22