



P Fridge backup

2025/12/1 09:59:57

Device

Type of device KH 50	Serial n° OK 17.12.19808	Software version 1.06
-------------------------	-----------------------------	--------------------------


Dataset parameters

Dataset name P Fridge backup	Type of dataset Instant
Number of points 5856	Interval 15 minute(s)
Start date 2025/10/1 10:05:00	End date 2025/12/1 09:50:00

Comments

Channels

Channel Ch-int1 [°C]	Measure Temperature	Probe Ambient thermo-hygro		
Low threshold 2.0	High threshold 8.0			
Minimum 3.1	Maximum 5.4	Average 4.28	Standard 0.46	MKT 4.29

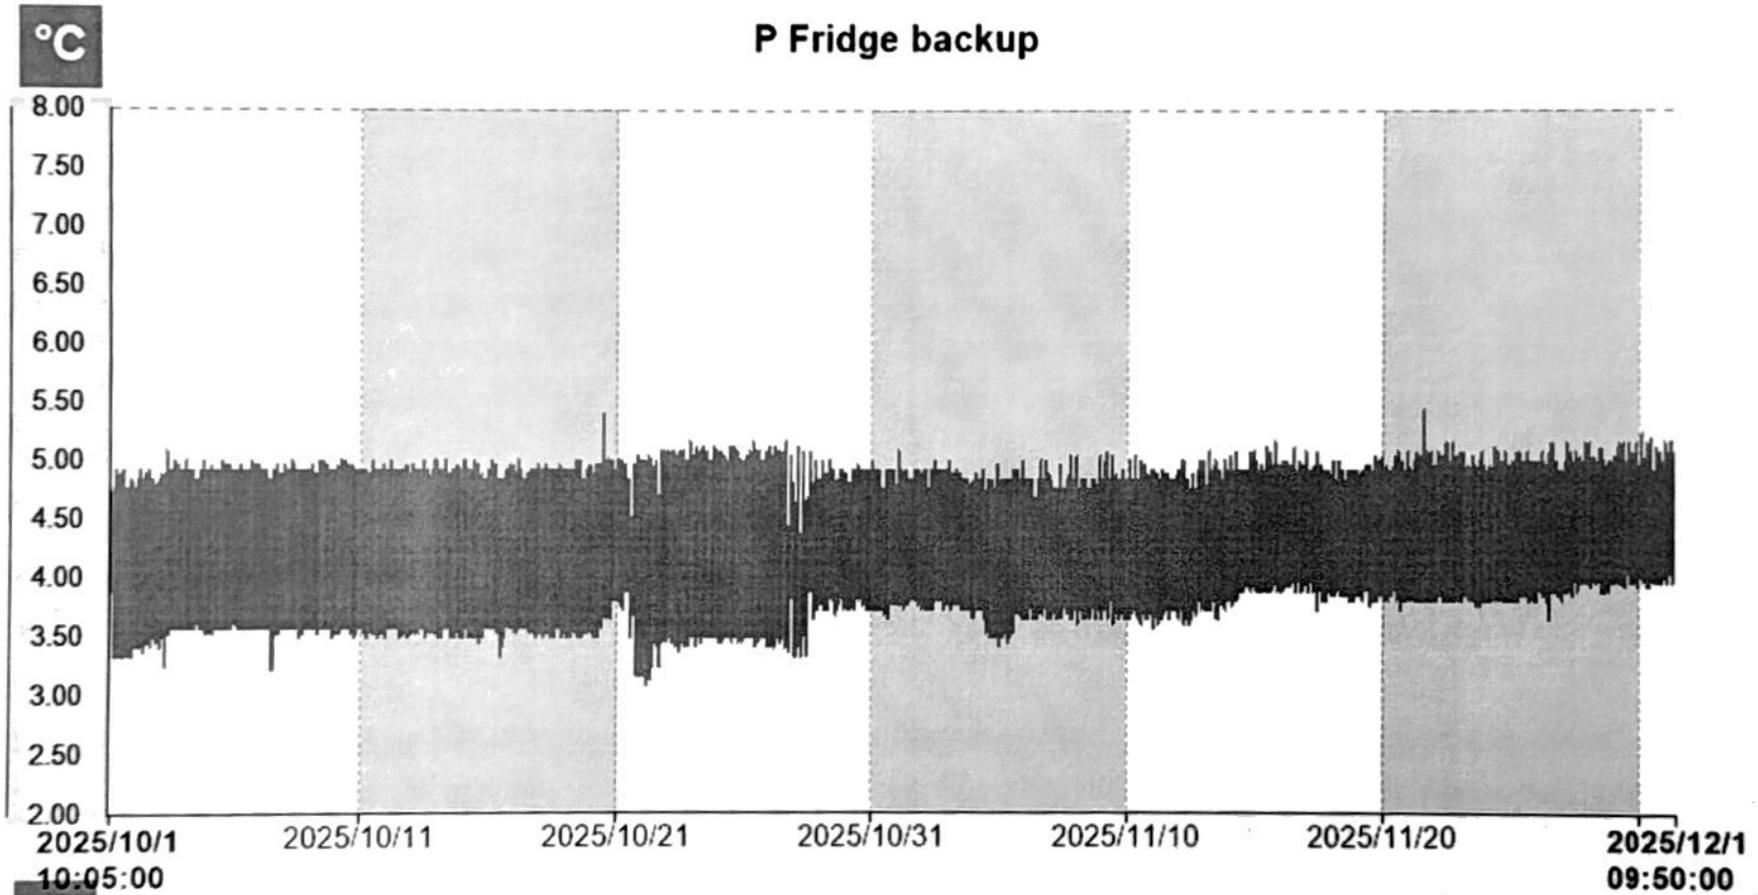



P Fridge backup
2025/12/1 09:59:57

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 17.12.19808] Ch-int1 [C]	5856	3.1	5.4	4.28	0.46	4.29