



P-Fridge
2026/1/2 11:14:44

Device

Type of device KH 50	Serial n° 0K 16.12.12000	Software version 1.06
-------------------------	-----------------------------	--------------------------

Dataset parameters


Dataset name P-Fridge	Type of dataset Instant
Number of points 5762	Interval 15 minute(s)
Start date 2025/11/3 10:50:00	End date 2026/1/2 11:05:00

Comments

Channels

Channel Ch-int1 [°C]	Measure Temperature	Probe Ambient thermo-hygro		
Low threshold 2.0	High threshold 8.0			
Minimum 3.0	Maximum 5.6	Average 4.11	Standard 0.47	MKT 4.13

2025/11/13
2025/11/23
2025/12/3
2025/12/13
2025/12/23
2026/1/2

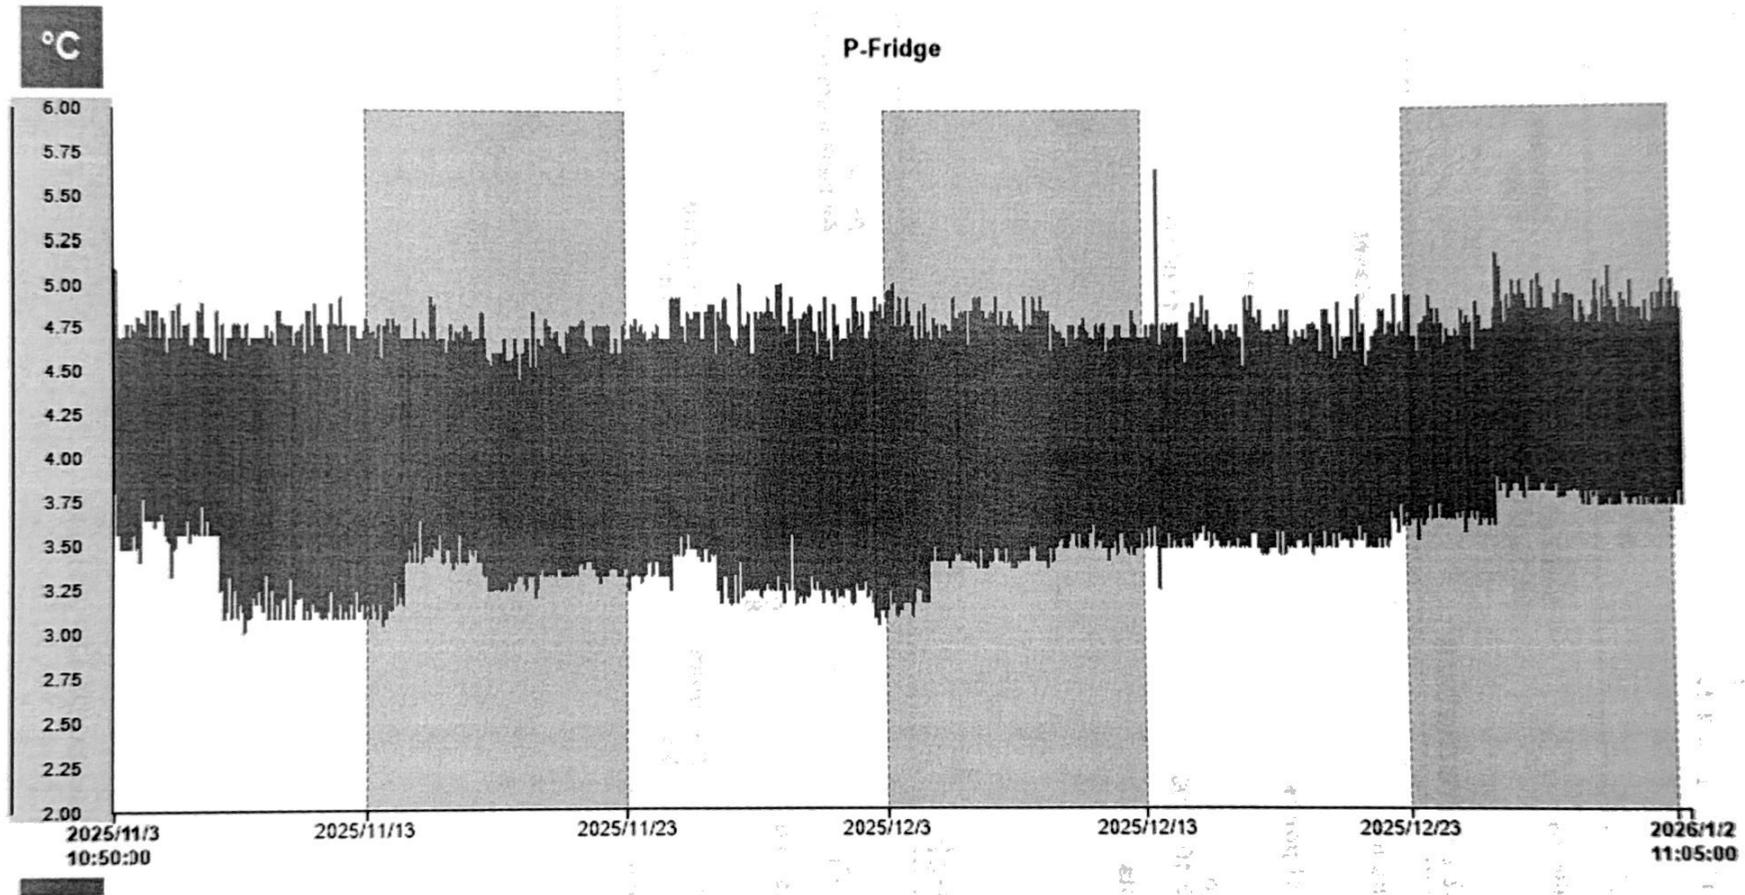



P-Fridge
2026/1/2 11:14:44

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.12.12000] Ch-int1 [°C]	5762	3.0	5.6	4.11	0.47	4.13