



**P-Fridge**  
2026/3/2 09:47:21

## Device

---

Type of device KH 50	Serial n° OK 16.12.12000	Software version 1.06
-------------------------	-----------------------------	--------------------------

## Dataset parameters

---


Dataset name P-Fridge	Type of dataset Instant
Number of points 5657	Interval 15 minute(s)
Start date 2026/1/2 11:40:00	End date 2026/3/2 09:40:00
Comments	

## Channels

---

Channel Ch-int1 [°C]	Measure Temperature	Probe Ambient thermo-hygro		
Low threshold 2.0	High threshold 8.0			
Minimum 3.4	Maximum 5.6	Average 4.42	Standard 0.41	MKT 4.43

---

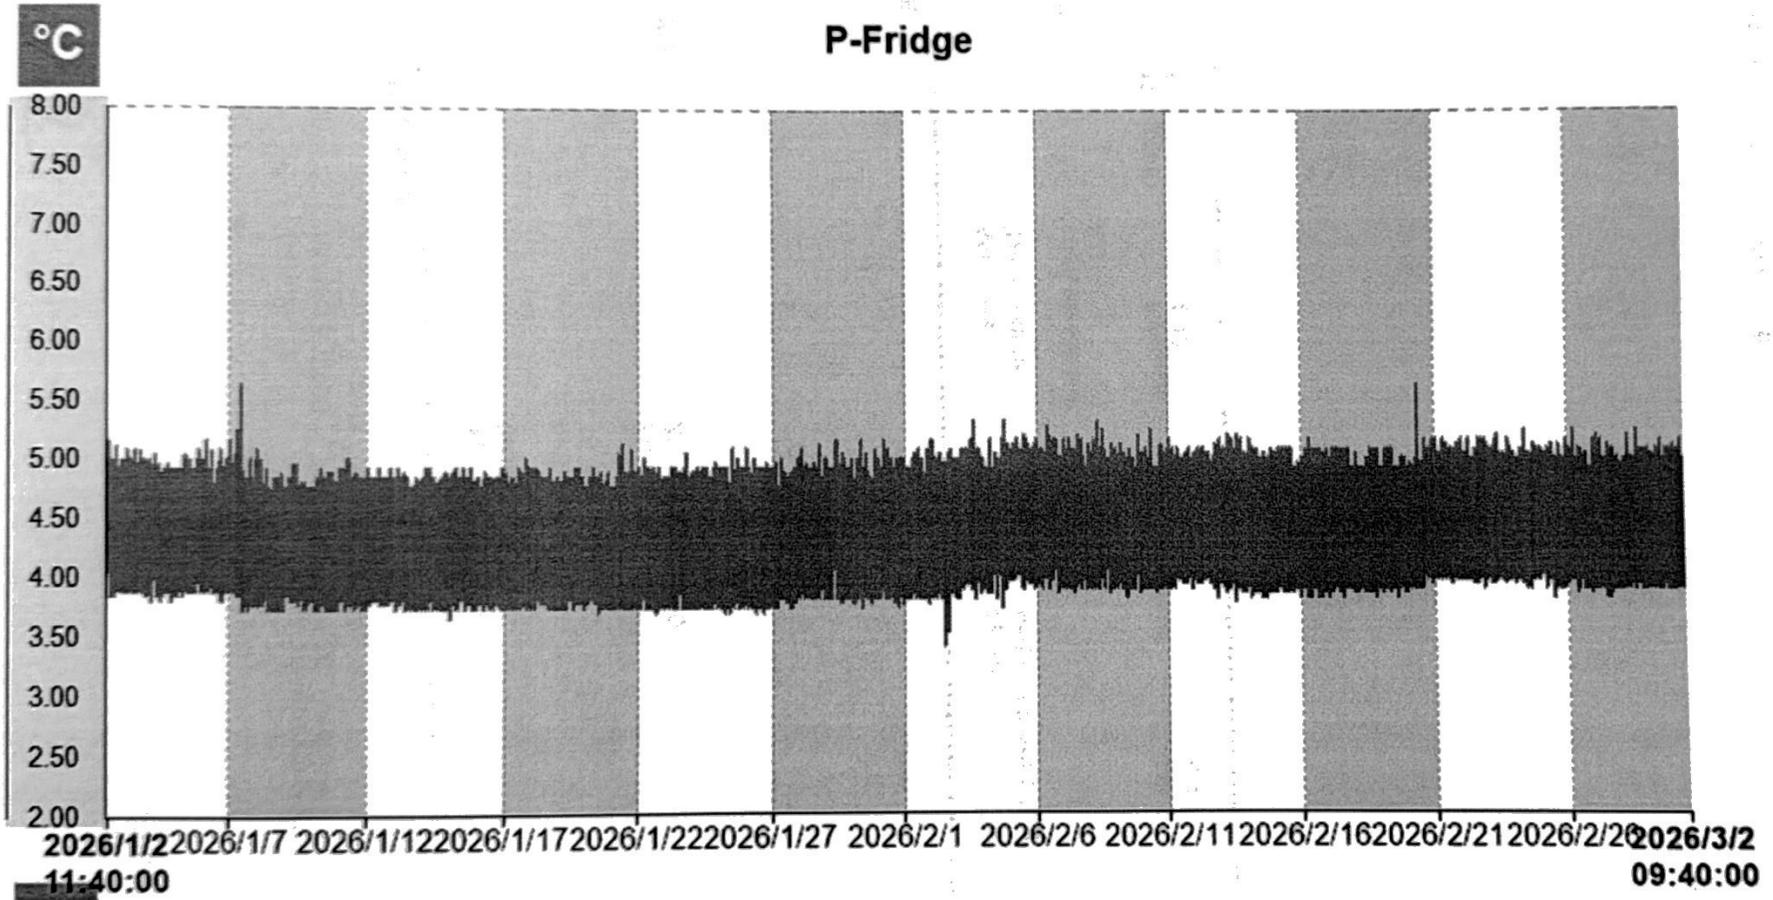

2026-1-17  
2026-1-17



**P-Fridge**  
2026/3/2 09:47:21

	<b>Number of points</b>	<b>Minimum</b>	<b>Maximum</b>	<b>Average</b>	<b>Standard deviation</b>	<b>MKT</b>
<b>KH 50 [OK 16.12.12000]</b> Ch-int1 [°C]	5657	3.4	5.6	4.42	0.41	4.43