



P Fridge backup

2026/2/2 08:32:24

Device

Type of device KH 50	Serial n° OK 17.12.19808	Software version 1.06
-------------------------	-----------------------------	--------------------------


Dataset parameters

Dataset name P Fridge backup	Type of dataset Instant
Number of points 6040	Interval 15 minute(s)
Start date 2025/12/1 10:35:00	End date 2026/2/2 08:20:00

Comments

Channels

Channel Ch-int1 [°C]	Measure Temperature	Probe Ambient thermo-hygro
Low threshold 2.0	High threshold 8.0	
Minimum 3.6	Maximum 5.8	Average 4.57
		Standard 0.38
		MKT 4.58

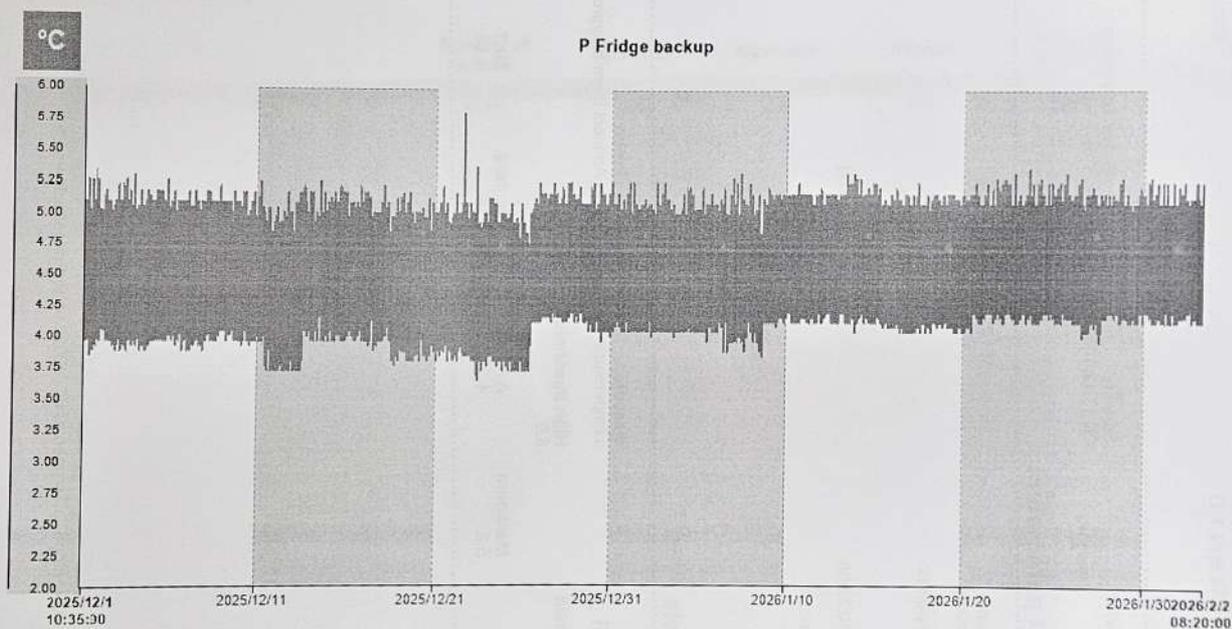



P Fridge backup

2026/2/2 08:32:25

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 17.12.19808] Ch-int1 [°C]	6040	3.6	5.8	4.57	0.38	4.58