



ROOM
2024/8/1 16:03:16

Device

Type of device	Serial n°	Software version
KH 50	OK 16.12.12003	1.06

Dataset parameters

Dataset name	Type of dataset
ROOM	Instant
Number of points	Interval
2615	15 minute(s)
Start date	End date
2024/7/5 10:25:00	2024/8/1 15:55:00
Comments	

Channels

Channel Ch-int1 [°C]		Measure Temperature	Probe Ambient thermo-hygro	
Low threshold 15.0		High threshold 25.0		
Minimum 20.8	Maximum 21.9	Average 21.54	Standard 0.18	MKT 21.54
.....				
Channel Ch-int2 [%RH]		Measure Hygrometry	Probe Ambient thermo-hygro	
Low threshold ---		High threshold ---		
Minimum 60.4	Maximum 62.5	Average 61.16	Standard 0.21	MKT 0.00
.....				




INSTRUMENTS

ROOM
2024/8/1 16:03:16

°C

ROOM

%RH

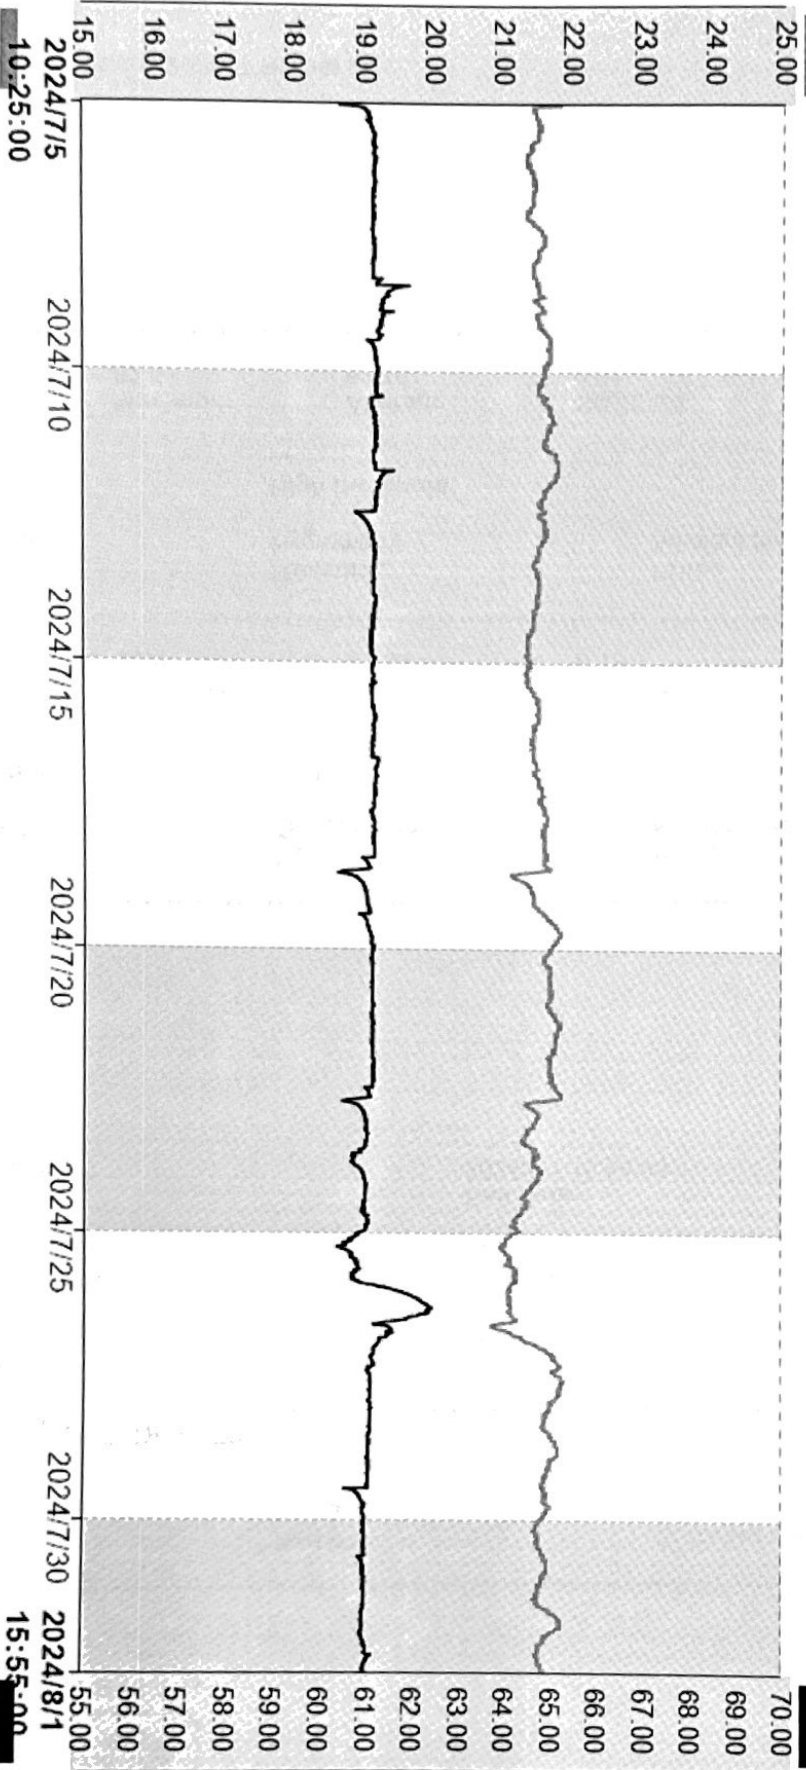

C:\Users\USER\Desktop\202407 ROOM.kfk



ROOM
2024/8/1 16:03:16

	Number of points	Minimum	Maximum	Average	Standard deviation	MKT
KH 50 [OK 16.12.12003]						
Ch-int1 [C]	2615	20.8	21.9	21.54	0.18	21.54
Ch-int2 [%RH]	2615	60.4	62.5	61.16	0.21	—